



*We flex to your specs*

2010-2011

INORGANIC STANDARDS & CUSTOM SOLUTIONS



Welcome to our 2010-2011 Catalog!

We are very excited at Inorganic Ventures about a number of things that we would like to share with you.

- Inorganic Ventures' official Ribbon Cutting Ceremony on October 14, 2009 marked the completion of our corporate relocation from Lakewood, New Jersey to Christiansburg, Virginia.
- On March 1, 2010 we'll be launching our new website. This will bring you online shopping improvements and a more user-friendly layout.
- In this very catalog, we've launched more than 75 new products designed to make your job easier:
  - Several new ICP-MS single element CRMs (beginning on page 12).
  - Rh in a nitric acid matrix with no trace chloride present (page 16).
  - 10,000 µg/mL Th and U CRMs (page 20).
  - Thirty-five new off-the-shelf instrument set-up, tuning and calibration solutions for your model of ICP-OES or ICP-MS (pages 26-33).
  - Three new ion chromatography CRMs (page 58).
  - Five new conductivity CRMs as low as 2 µmhos/cm (page 78).
  - A new line of pH buffers covering every pH from 2 thru 12 (pg 79).

We continue to place a strong emphasis on customer satisfaction. In that spirit, we've added several new chemists to our team who are looking forward to working with you.

In closing, I'd like to personally thank you for choosing Inorganic Ventures as your CRM manufacturer. We look forward to serving your needs in the years to come.

Paul R. Gaines, Ph.D.  
CEO & Fellow Chemist  
Serving You in Chemistry



## Dedicated...

I was given the task of developing a sample prep method for a unique suds suppressor material. Inorganic Ventures' Dr. Gaines was very helpful and was willing to spend what I considered significant consultation time with me on the phone, which saved me a bundle of time researching information through other sources.

*Tim Mills*  
Cincinnati, OH

|   |                |
|---|----------------|
| <b>WE FLEX TO YOUR SPECS.....</b>             | <b>2</b>       |
| ■ Inorganics, Customs & More .....            | 2-3            |
| ■ Product Documentation.....                  | 4              |
| ■ Technical Support.....                      | 5              |
| ■ Refunds & Replacements.....                 | 6              |
| <b>CUSTOM STANDARDS .....</b>                 | <b>7</b>       |
| ■ Trust the Specialists .....                 | 8              |
| ■ Flexing to Your Specs .....                 | 9              |
| ■ Easy as 1, 2, 3.....                        | 10             |
| ■ Quotation Request Form .....                | 89             |
| <b>ICP &amp; ICP-MS .....</b>                 | <b>11</b>      |
| ■ Single-Element Standards.....               | 12-20          |
| ■ Isotopic Standards.....                     | 21             |
| ■ Speciation Standards.....                   | 22             |
| ■ Cyanide Standards.....                      | 22             |
| ■ Multi-Element Standards.....                | 23-33          |
| ■ High-Purity Ionization Buffers.....         | 34             |
| ■ EPA Standards.....                          | 34-56          |
| ■ Custom ICP Standards.....                   | see pages 7-10 |
| <b>ION CHROMATOGRAPHY .....</b>               | <b>57</b>      |
| ■ Anion Standards.....                        | 58-59          |
| ■ Cation Standards.....                       | 60             |
| ■ Multi-Ion Standards.....                    | 61             |
| ■ Eluent Concentrates.....                    | 61             |
| ■ EPA Standards.....                          | 62-64          |
| ■ Custom IC Standards.....                    | see pages 7-10 |
| <b>ATOMIC ABSORPTION .....</b>                | <b>65</b>      |
| ■ Single-Element Standards.....               | 66-68          |
| ■ Modifiers, Buffers & Releasing Agents.....  | 69             |
| ■ Multi-Element Standards.....                | 69             |
| ■ EPA Standards.....                          | 70             |
| ■ Custom AA Solutions.....                    | see pages 7-10 |
| <b>WATER QC.....</b>                          | <b>71</b>      |
| ■ Potable Water Standards.....                | 72-73          |
| ■ Wastewater Standards.....                   | 74-76          |
| ■ Custom QC Standards.....                    | see pages 7-10 |
| <b>WET CHEMISTRY .....</b>                    | <b>77</b>      |
| ■ Wet Chemical Standards.....                 | 78             |
| ■ Sample Preparation.....                     | 79-81          |
| ■ Custom Wet Chemistry Solutions.....         | see pages 7-10 |
| ■ Real World Reference Materials by RTC.....  | 82             |
| ■ Ordering, Terms & Conditions.....           | 84             |
| ■ Index by Subject.....                       | 85             |
| ■ Index by Catalog Number.....                | 86-88          |
| ■ Custom Standard Quotation Request Form..... | 89             |



*We flex to your specs.* That's not just our motto—it's what we do. Inorganic Ventures is known for producing exactly what you need, when you need it. Others might come close to our quality, but no one can match our flexibility. We're small enough to avoid the bottlenecks that slow other suppliers. And since we're smaller, you'll always get support from a live person—never a computer. Yet we're big enough to have the manpower and facilities to create nearly any inorganic standard.

In every aspect of our business, from fast, friendly service to product customization, *we flex to your specs.*

## Inorganics

*A history of accreditation.* For nearly a decade, Inorganic Ventures has been registered to the three most important ISO certifications for Certified Reference Material producers (see right). Both A2LA and QMI have accredited our laboratory, giving you complete confidence in our standards. We've been registered to ISO Guide 34:2000, General Requirements for the Competence of Reference Materials Producers, longer than any other inorganic standards manufacturer. So you can rest easy knowing that our CRMs are:

- **Traceable**

We use NIST Standard Reference Materials (SRM and lot number specified on the certificate) for calibration and direct comparison.

- **Precise**

We have detailed Error Budgets that define the errors used in determining the uncertainty, giving us a unique value for each lot of material.

- **Pure**

We use ICP and ICP-MS to check the purity of all CRMs. Protocols are prepared for all new starting materials. We perform purifications and chemical modifications as required to meet predefined quality specifications.

- **Accurate**

We use two independent validated assay methods that are performed with a reliable QC standard.

- **Stable & Compatible**

We've conducted stability studies on all standards, including blends. Compatibility and stability have been demonstrated and fully documented.



### Innovative...

When they say, "We flex to your specs," they aren't kidding! Inorganic Ventures custom-made products for us that exceeded our expectations and were as well thought out, unique, and innovative as our mercury analyzers.

*Philip Dufresne  
Cleveland, OH*

## Customs

**Fast, credible, cooperative.** Whether you need two analytes or twenty, milliliters or liters, 0.001 µg/mL or 10,000, we can make it for you—fast.

- Price quotes in hours, not days
- 99% ship in five business days or less
- Next-day RUSH manufacturing—at no additional cost

See page 8 to learn more.

### Flexible...

Inorganic Ventures has been flexible in providing us custom-blended ICP standards for about eight years. You guys have even reported the concentrations in a different format that suits our needs and makes it much easier for our analysts.

*Floyd Myers  
 Blacksburg, SC*

## And More...

**On the web.** As one of our customers, it's important to us that you succeed. In that spirit, we invite you to visit our website at [www.inorganicventures.com](http://www.inorganicventures.com) where you'll find several indispensable tools for conducting your lab work. *Look for our new website coming March of 2010!*

**Analytical Periodic Table**  
 Discover the best online tool for analytical chemists. Includes chemical compatibilities, preferred lines, major interferences, and additional data for 70+ elements.  
[www.inorganicventures.com/extras/pertable](http://www.inorganicventures.com/extras/pertable)

**ICP Operations Guide**  
 A 16-part online guide intended for anyone preparing samples and standards for measurement using ICP. Topics cover many day-to-day tasks required by all operators.  
[www.inorganicventures.com/tech/icp-ops](http://www.inorganicventures.com/tech/icp-ops)

**Reliable Measurements Guide**  
 An essential 17-part online guide for chemical analysts. Topics cover all phases of sample collection, preparation, measurement, and data analysis.  
[www.inorganicventures.com/tech/reliability](http://www.inorganicventures.com/tech/reliability)


**Sample Preparation Guide**  
 This expanding online guide features dozens of elements. Each part includes detailed preparation and solution chemistry for samples containing the element of interest.  
[www.inorganicventures.com/tech/samprep](http://www.inorganicventures.com/tech/samprep)

**In the lab.** Your inorganic analyses are supported every step of the way. The product documentation supplied with every standard can be referenced for traceability, impurities and certified values (see page 4). And our technical support is always available should you need a hand (see page 5).



**Certificates of Analysis.** Our certificates probably show a lot more data than you're used to seeing, and with good reason. As a tri-tier ISO registered manufacturer, our certificates follow strict international guidelines. This ensures that they include extensive data to meet the quality prerequisites of any laboratory.

- **Traceable** - to specific NIST SRMs and lots.
- **Certified values** - based on two independent methods.
- **Trace impurities** - listed with the actual values.

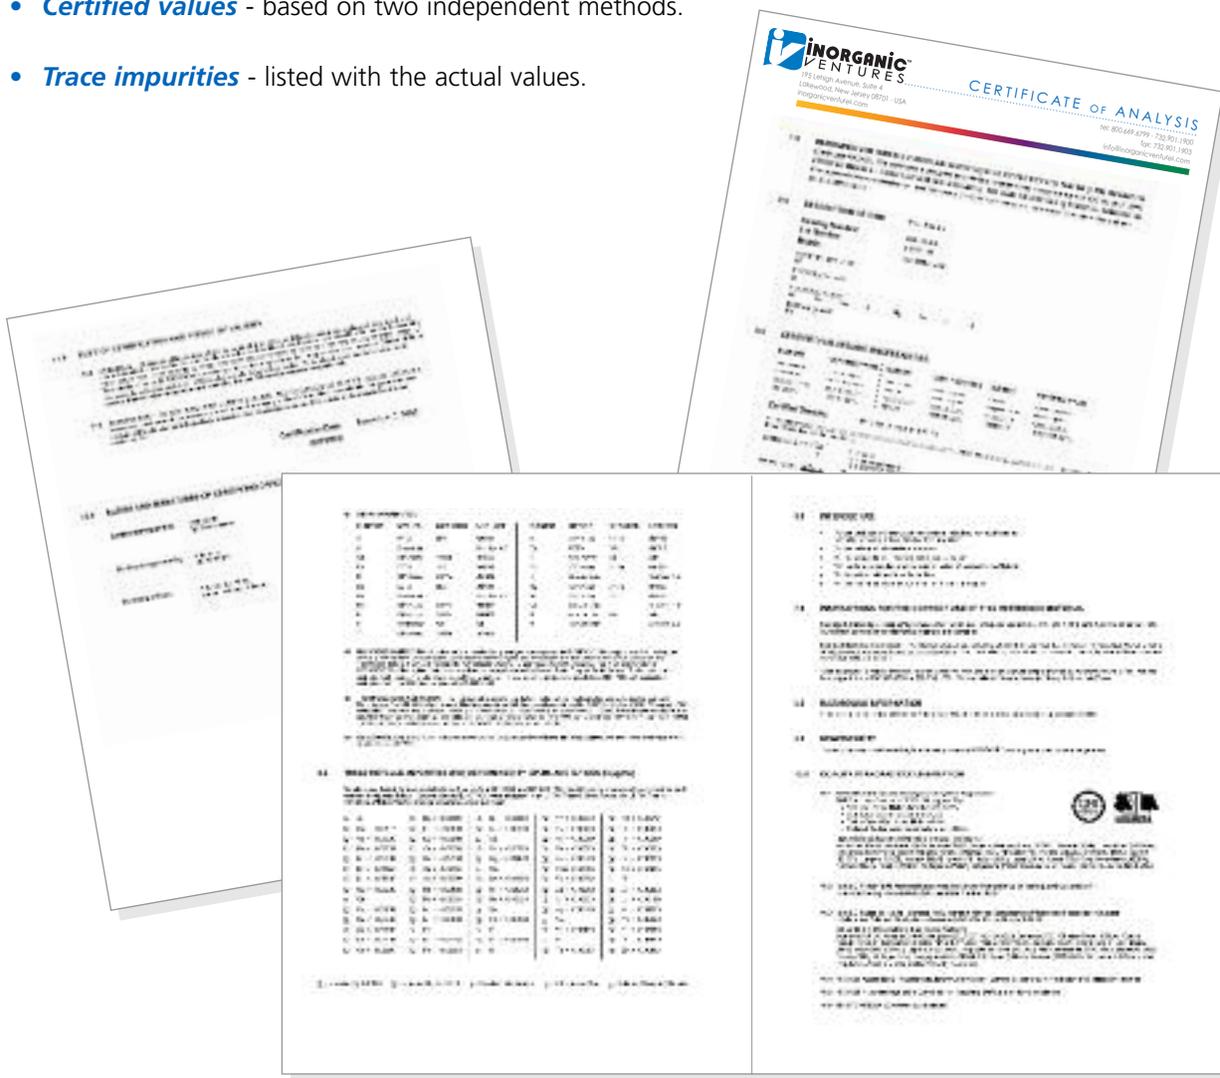

You'll wonder how you ever got along without such a thorough certificate.  
[Contact us for a sample.](#)

**Material Safety Data Sheets.** Our EU-compliant 16-part MSDS format also complies with WHMIS standards for our Canadian and European customers. For samples and replacements, see our website.

*We're here to help.* Whether you need detailed assistance or quick troubleshooting, our expertise is yours for the asking. We can assist you with hundreds of topics ranging from problem elements to calculations. Technical advisors are available Monday through Friday from 8:00 AM – 6:00 PM (EST).

## Phone

- 1.800.669.6799 (US & Canada)
- 1.540.585.3030 (International)

## Email

- [info@inorganicventures.com](mailto:info@inorganicventures.com)

## Online

- [www.inorganicventures.com](http://www.inorganicventures.com)



## Tech Tips

1. Don't put pipettes directly into your standard bottles. Pour some of the standard into a disposable plastic container, remove your aliquot, and then discard the remainder.
2. Weigh your standard before storage and then just before its next use. The weight will decrease if there is significant transpiration.
3. Never use glass pipettes or transfer devices with standards containing HF. Free HF attacks glass.

*Get more technical advice at [www.inorganicventures.com](http://www.inorganicventures.com)!*




## We can assist you with...

- Sample preparation
- Spectral interferences
- Chemical compatibilities
- Various ICP & ICP-MS measurement issues

WE FLEX TO YOUR SPECS  
**REFUNDS & REPLACEMENTS**

*Unquestionable integrity.* Every order that leaves our facility includes our *Declaration of Integrity*. This document guarantees, in no uncertain terms, if you're dissatisfied with your order for any reason, we'll bend over backwards to make it right.

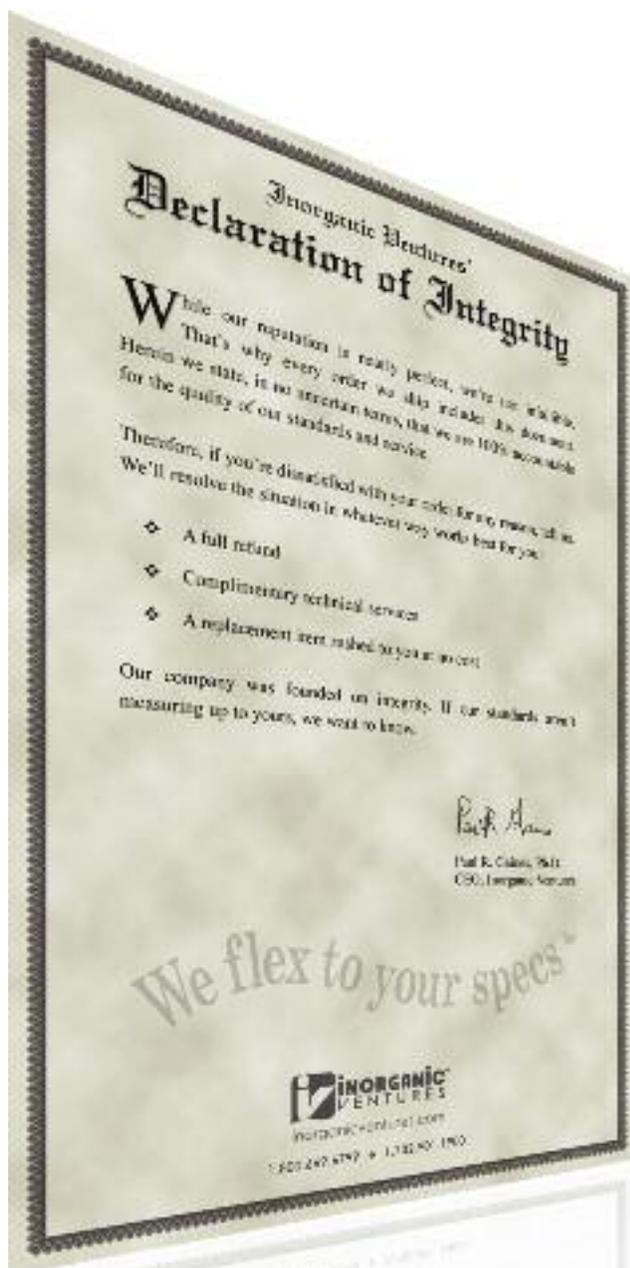

### Committed...

We actually have Inorganic Ventures' Declaration of Integrity hanging up on our bulletin board in our office as a reminder for ourselves to provide the highest quality of service. We wouldn't think of switching to another vendor.

*James Piper*  
Mechanicsburg, PA



## Speed. Credibility. Cooperation.

We can prepare almost any inorganic blend within the boundaries of science. Whether you need two analytes or twenty, milliliters or liters, 0.001  $\mu\text{g/mL}$  or 10,000, we can make it for you — fast. It's our specialty.

**Customization** — The most prominent way that we flex to your specs.

## Contents

|                             |    |
|-----------------------------|----|
| Trust the Specialists ..... | 8  |
| Flexing to Your Specs ..... | 9  |
| Easy as 1, 2, 3 .....       | 10 |
| Quotation Request Form..... | 89 |

- ✓ **Traceable to NIST SRMs and lots**
- ✓ **Produced under ISO Guide 9001:2000**
- ✓ **Produced under ISO Guide 17025:2005**
- ✓ **Produced under ISO Guide 34:2000**
- ✓ **Assayed by optimal validated procedure**



CUSTOM STANDARDS  
TRUST THE SPECIALISTS



## If they were this easy, we'd be out of a job.

But custom blending isn't easy. It takes a specialist to do it well. And Inorganic Ventures is the only manufacturer to specialize in custom inorganic standards. We don't just make them your way, we make them the best way. Every solution is engineered to be stable, compatible and easy to use. And we make them fast—99% ship in five business days or less.

Next time you need a custom inorganic standard, contact Inorganic Ventures—*we flex to your specs.*



Our catalog reveals only a fraction of the inorganic solutions we're able to make. Much of our business is devoted entirely to custom blending. Laboratories in more than 50 countries trust us exclusively to manufacture their inorganic standards.



### Fast

Our specialization in custom blending means faster service, without sacrificing quality. Our experienced technicians can identify stability and compatibility issues before production even begins. Almost every blend we make is prepared, certified and shipped in five business days or less.



### Credible

Since 1999, our tri-tier ISO quality system has ensured that every standard we make is engineered to be stable, compatible and easy to use. These international accreditations guarantee that you're receiving a true Certified Reference Material.

- [ISO Guide 34](#) ensures the reliability of our reference materials.
- [ISO/IEC 17025](#) ensures the competency of our laboratory.
- [ISO 9001:2008](#) ensures the quality of our services.



### Cooperative

Speed and credibility often come at a higher price. But you'd be surprised how elastic that price can be. We offer specialized purchasing options and other incentives to better accommodate any budget. Just ask. We're happy to manufacture nearly any solution in bulk quantities. This prevents the need for repeat labor, which means you'll save money. Plus, there's no waiting when you reorder the material—it'll ship the day you order.

### Dependable...


Inorganic Ventures has been a super-dependable source of our custom calibration standards for ICP-MS. We have a succinct set of customs that are efficient to use, dependable and long-lasting. Inorganic Ventures is a big part of backing up our company motto: "Numbers you can count on."

*Jeff Yoshimoto  
Sparks, NV*



## Request your solutions.

Generate and request any number of custom solutions at [inorganicventures.com](http://inorganicventures.com). Or, call in your request to 1.800.669.6799 and discuss your needs with a specialist. You may also fax the quotation request form found on page 89.



## Review our quotation.

Often you'll receive our pricing in less than two hours. If you like what you see, place your order by phone, fax or web. However, if you're not happy with our quoted price, let us know. We may be able to better accommodate your budget.



## Receive your order.

99% of the custom orders we prepare ship in five business days or less. If we expect it to take longer, we'll let you know. When your need is truly urgent, we offer next-day RUSH manufacturing\* at no additional charge—just ask.

Plus, everything we make is backed by our Declaration of Integrity (see page 6). Your satisfaction is 100% guaranteed for the lifetime of the solution.

### Time-saving...

Because of our laboratory's broad calibration ranges, Inorganic Ventures has always been able to prepare wide-ranging calibration solutions for our particular operations. These customized solutions save us time and money and simplify our preparatory work considerably.

*Mark Ellison  
San Jose, CA*



\* 48-72 hour arrival time when you specify RUSH manufacturing.



Whether you use ICP or ICP-MS, we offer a wide selection of certified reference materials. At your request, we've expanded our line with more 500 mL sizes of 10,000 µg/mL standards and new instrument setup standards. And we'll continue to improve our selection based on your feedback.

**User-Driven Development** — Another fundamental way in which we flex to your specs.

## Contents

|                                      |                |
|--------------------------------------|----------------|
| Single-Element Standards .....       | 12-20          |
| Isotopic Standards .....             | 21             |
| Speciation Standards .....           | 22             |
| Cyanide Standards .....              | 22             |
| Multi-Element Standards .....        | 23-33          |
| High Purity Ionization Buffers ..... | 34             |
| EPA Standards.....                   | 34-56          |
| Custom ICP Standards.....            | see pages 7-10 |

- ✓ **Traceable to NIST SRMs and lots**
- ✓ **Produced under ISO Guide 9001:2000**
- ✓ **Produced under ISO Guide 17025:2005**
- ✓ **Produced under ISO Guide 34:2000**
- ✓ **Assayed by validated Wet Chemical procedures**
- ✓ **Assayed by validated ICP-OES procedures**
- ✓ **Trace metallic impurities determined by ICP and ICP-MS**



10 µg/mL

## 10 µg/mL Standards

Custom 10 µg/mL standards are available upon request.

NEW

NEW

NEW

NEW

NEW

NEW

NEW

| Analyte                                   | Matrix                                   | Starting Material   | Volume | Catalog #   |
|---|--|---|--------|-------------|
| Aluminum, Al                              | HNO <sub>3</sub>                         | Al metal  | 125 mL | MSAL-10PPM  |
| Antimony, Sb                              | HNO <sub>3</sub> / Tartaric              | Sb metal  | 125 mL | MSSB-10PPM  |
| Arsenic, As                               | HNO <sub>3</sub>                         | As metal  | 125 mL | MSAS-10PPM  |
| Barium, Ba                                | HNO <sub>3</sub>                         | Ba(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | MSBA-10PPM  |
| Beryllium, Be                             | HNO <sub>3</sub>                         | Be <sub>4</sub> O(C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> ) <sub>6</sub> | 125 mL | MSBE-10PPM  |
| Bismuth, Bi                               | HNO <sub>3</sub>                         | Bi metal  | 125 mL | MSBI-10PPM  |
| Boron, B                                  | H <sub>2</sub> O                         | H <sub>3</sub> BO <sub>3</sub>  | 125 mL | MSB-10PPM   |
| Cadmium, Cd                               | HNO <sub>3</sub>                         | Cd metal  | 125 mL | MSCD-10PPM  |
| Calcium, Ca                               | HNO <sub>3</sub>                         | CaO   | 125 mL | MSCA-10PPM  |
| Cerium, Ce                                | HNO <sub>3</sub>                         | CeO <sub>2</sub>  | 125 mL | MSCE-10PPM  |
| Cesium, Cs                                | HNO <sub>3</sub>                         | CeO <sub>2</sub>  | 125 mL | MSCS-10PPM  |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup> | HNO <sub>3</sub>                         | Cr metal  | 125 mL | MSCR3-10PPM |
| Chromium <sup>+6</sup> , Cr <sup>+6</sup> | H <sub>2</sub> O                         | (NH <sub>4</sub> ) <sub>2</sub> Cr <sub>2</sub> O <sub>7</sub>                | 125 mL | MSCR6-10PPM |
| Cobalt, Co                                | HNO <sub>3</sub>                         | Co metal  | 125 mL | MSCO-10PPM  |
| Copper, Cu                                | HNO <sub>3</sub>                         | Cu metal  | 125 mL | MSCU-10PPM  |
| Germanium, Ge                             | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Ge metal  | 125 mL | MSGE-10PPM  |
| Gold, Au                                  | HCl                                      | AuCl <sub>3</sub>   | 125 mL | MSAU-10PPM  |
| Hafnium, Hf                               | H <sub>2</sub> O / HNO <sub>3</sub> / HF | HfO <sub>2</sub>  | 125 mL | MSHF-10PPM  |
| Holmium, Ho                               | HNO <sub>3</sub>                         | Ho <sub>2</sub> O <sub>3</sub>  | 125 mL | MSHO-10PPM  |
| Indium, In                                | HNO <sub>3</sub>                         | In metal  | 125 mL | MSIN-10PPM  |
| Iron, Fe                                  | HNO <sub>3</sub>                         | Fe metal  | 125 mL | MSFE-10PPM  |
| Lead, Pb                                  | HNO <sub>3</sub>                         | Pb(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | MSPB-10PPM  |
| Lithium, Li                               | HNO <sub>3</sub>                         | Li <sub>2</sub> CO <sub>3</sub>   | 125 mL | MSLI-10PPM  |
| <sup>6</sup> Lithium, <sup>6</sup> Li     | HNO <sub>3</sub>                         | <sup>6</sup> Li metal   | 125 mL | MS6LI-10PPM |
| Magnesium, Mg                             | HNO <sub>3</sub>                         | Mg metal  | 125 mL | MSMG-10PPM  |
| Manganese, Mn                             | HNO <sub>3</sub>                         | Mn metal  | 125 mL | MSMN-10PPM  |
| Mercury, Hg                               | HCl                                      | Hg metal  | 125 mL | MSHG-10PPM  |
| Mercury, Hg                               | HNO <sub>3</sub>                         | Hg metal  | 125 mL | MSHGN-10PPM |
| Molybdenum, Mo                            | H <sub>2</sub> O / NH <sub>4</sub> OH    | (NH <sub>4</sub> ) <sub>2</sub> MoO <sub>4</sub>                              | 125 mL | MSMO-10PPM  |
| Nickel, Ni                                | HNO <sub>3</sub>                         | Ni metal  | 125 mL | MSNI-10PPM  |
| Osmium, Os                                | HCl                                      | (NH <sub>4</sub> ) <sub>2</sub> OsCl <sub>6</sub>                             | 125 mL | MSOS-10PPM  |
| Phosphorus, P                             | H <sub>2</sub> O                         | H <sub>3</sub> PO <sub>4</sub>  | 125 mL | MSP-10PPM   |
| Platinum, Pt                              | HCl                                      | Pt Metal  | 125 mL | MSPT-10PPM  |
| Potassium, K                              | HNO <sub>3</sub>                         | KNO <sub>3</sub>  | 125 mL | MSK-10PPM   |
| Rhodium, Rh                               | HCl                                      | RhCl <sub>3</sub>   | 125 mL | MSRH-10PPM  |
| Rhodium, Rh                               | HNO <sub>3</sub>                         | RhNO <sub>3</sub>   | 125 mL | MSRHN-10PPM |
| Scandium, Sc                              | HNO <sub>3</sub>                         | Sc <sub>2</sub> O <sub>3</sub>  | 125 mL | MSSC-10PPM  |
| Selenium, Se                              | HNO <sub>3</sub>                         | Se metal  | 125 mL | MSSE-10PPM  |
| Silicon, Si                               | H <sub>2</sub> O / HNO <sub>3</sub> / HF | SiO <sub>2</sub>  | 125 mL | MSSI-10PPM  |
| Silver, Ag                                | HNO <sub>3</sub>                         | Ag metal  | 125 mL | MSAG-10PPM  |
| Sodium, Na                                | HNO <sub>3</sub>                         | Na <sub>2</sub> CO <sub>3</sub>   | 125 mL | MSNA-10PPM  |
| Strontium, Sr                             | HNO <sub>3</sub>                         | SrCO <sub>3</sub>   | 125 mL | MSSR-10PPM  |
| Sulfur, S                                 | H <sub>2</sub> O                         | H <sub>2</sub> SO <sub>4</sub>  | 125 mL | MSS-10PPM   |
| Tellurium, Te                             | HNO <sub>3</sub>                         | Te Metal  | 125 mL | MSTEN-10PPM |
| Terbium, Tb                               | HNO <sub>3</sub>                         | Tb <sub>4</sub> O <sub>7</sub>  | 125 mL | MSTB-10PPM  |
| Thallium, Tl                              | HNO <sub>3</sub>                         | TlNO <sub>3</sub>   | 125 mL | MSTL-10PPM  |
| Thorium, Th                               | HNO <sub>3</sub>                         | Th(NO <sub>3</sub> ) <sub>4</sub> ·xH <sub>2</sub> O                          | 125 mL | MSTH-10PPM  |
| Tin, Sn                                   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Sn metal  | 125 mL | MSSN-10PPM  |
| Titanium, Ti                              | HNO <sub>3</sub> / HF                    | Ti metal  | 125 mL | MSTI-10PPM  |
| Tungsten, W                               | HNO <sub>3</sub> / HF                    | W Metal   | 125 mL | MSW-10PPM   |
| Uranium, U                                | HNO <sub>3</sub>                         | UO <sub>2</sub> (NO <sub>3</sub> ) <sub>2</sub>                               | 125 mL | MSU-10PPM   |
| Vanadium, V                               | HNO <sub>3</sub>                         | V <sub>2</sub> O <sub>5</sub>   | 125 mL | MSV-10PPM   |
| Yttrium, Y                                | HNO <sub>3</sub>                         | Y <sub>2</sub> O <sub>3</sub>   | 125 mL | MSY-10PPM   |
| Zinc, Zn                                  | HNO <sub>3</sub>                         | Zn metal  | 125 mL | MSZN-10PPM  |

## SINGLE-ELEMENT STANDARDS

## 100 µg/mL Standards

Custom 100 µg/mL standards are available upon request.

100 µg/mL

| Analyte  | Matrix                                   | Starting Material   | Volume | Catalog #    |
|--|--|---|--------|--------------|
| Aluminum, Al   | HNO <sub>3</sub>                         | Al metal  | 125 mL | MSAL-100PPM  |
| Antimony, Sb   | HNO <sub>3</sub> / Tartaric              | Sb metal  | 125 mL | MSSB-100PPM  |
| Arsenic, As  | HNO <sub>3</sub>                         | As metal  | 125 mL | MSAS-100PPM  |
| Barium, Ba   | HNO <sub>3</sub>                         | Ba(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | MSBA-100PPM  |
| Beryllium, Be  | HNO <sub>3</sub>                         | Be <sub>4</sub> O(C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> ) <sub>6</sub> | 125 mL | MSBE-100PPM  |
| Bismuth, Bi  | HNO <sub>3</sub>                         | Bi metal  | 125 mL | MSBI-100PPM  |
| <b>NEW</b> Boron, B                                  | H <sub>2</sub> O                         | H <sub>3</sub> BO <sub>3</sub>  | 125 mL | MSB-100PPM   |
| Cadmium, Cd  | HNO <sub>3</sub>                         | Cd metal  | 125 mL | MSCD-100PPM  |
| Calcium, Ca  | HNO <sub>3</sub>                         | CaO   | 125 mL | MSCA-100PPM  |
| Cerium, Ce   | HNO <sub>3</sub>                         | CeO <sub>2</sub>  | 125 mL | MSCE-100PPM  |
| <b>NEW</b> Cesium, Cs                                | HNO <sub>3</sub>                         | CeO <sub>2</sub>  | 125 mL | MSCS-100PPM  |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup>            | HNO <sub>3</sub>                         | Cr metal  | 125 mL | MSCR3-100PPM |
| <b>NEW</b> Chromium <sup>+6</sup> , Cr <sup>+6</sup> | H <sub>2</sub> O                         | (NH <sub>4</sub> ) <sub>2</sub> Cr <sub>2</sub> O <sub>7</sub>                | 125 mL | MSCR6-100PPM |
| Cobalt, Co   | HNO <sub>3</sub>                         | Co metal  | 125 mL | MSCO-100PPM  |
| Copper, Cu   | HNO <sub>3</sub>                         | Cu metal  | 125 mL | MSCU-100PPM  |
| Germanium, Ge  | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Ge metal  | 125 mL | MSGE-100PPM  |
| Gold, Au   | HCl                                      | AuCl <sub>3</sub>   | 125 mL | MSAU-100PPM  |
| Hafnium, Hf  | H <sub>2</sub> O / HNO <sub>3</sub> / HF | HfO <sub>2</sub>  | 125 mL | MSHF-100PPM  |
| Holmium, Ho  | HNO <sub>3</sub>                         | Ho <sub>2</sub> O <sub>3</sub>  | 125 mL | MSHO-100PPM  |
| Indium, In   | HNO <sub>3</sub>                         | In metal  | 125 mL | MSIN-100PPM  |
| Iron, Fe   | HNO <sub>3</sub>                         | Fe metal  | 125 mL | MSFE-100PPM  |
| Lead, Pb   | HNO <sub>3</sub>                         | Pb(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | MSPB-100PPM  |
| Lithium, Li  | HNO <sub>3</sub>                         | Li <sub>2</sub> CO <sub>3</sub>   | 125 mL | MSLI-100PPM  |
| <sup>6</sup> Lithium, <sup>6</sup> Li                | HNO <sub>3</sub>                         | <sup>6</sup> Li metal   | 125 mL | MS6LI-100PPM |
| Magnesium, Mg  | HNO <sub>3</sub>                         | Mg metal  | 125 mL | MSMG-100PPM  |
| Manganese, Mn  | HNO <sub>3</sub>                         | Mn metal  | 125 mL | MSMN-100PPM  |
| Mercury, Hg  | HCl                                      | Hg metal  | 125 mL | MSHG-100PPM  |
| <b>NEW</b> Mercury, Hg                               | HNO <sub>3</sub>                         | Hg metal  | 125 mL | MSHGN-100PPM |
| Molybdenum, Mo                                       | H <sub>2</sub> O / NH <sub>4</sub> OH    | (NH <sub>4</sub> ) <sub>2</sub> MoO <sub>4</sub>                              | 125 mL | MSMO-100PPM  |
| <b>NEW</b> Nickel, Ni                                | HNO <sub>3</sub>                         | Ni metal  | 125 mL | MSNI-100PPM  |
| Osmium, Os   | HCl                                      | (NH <sub>4</sub> ) <sub>2</sub> OsCl <sub>6</sub>                             | 125 mL | MSOS-100PPM  |
| Phosphorus, P  | H <sub>2</sub> O                         | H <sub>3</sub> PO <sub>4</sub>  | 125 mL | MSP-100PPM   |
| Platinum, Pt   | HCl                                      | Pt Metal  | 125 mL | MSPT-100PPM  |
| Potassium, K   | HNO <sub>3</sub>                         | KNO <sub>3</sub>  | 125 mL | MSK-100PPM   |
| Rhodium, Rh  | HCl                                      | RhCl <sub>3</sub>   | 125 mL | MSRH-100PPM  |
| <b>NEW</b> Rhodium, Rh                               | HNO <sub>3</sub>                         | RhNO <sub>3</sub>   | 125 mL | MSRHN-100PPM |
| Scandium, Sc   | HNO <sub>3</sub>                         | Sc <sub>2</sub> O <sub>3</sub>  | 125 mL | MSSC-100PPM  |
| Selenium, Se   | HNO <sub>3</sub>                         | Se metal  | 125 mL | MSSE-100PPM  |
| Silicon, Si  | H <sub>2</sub> O / HNO <sub>3</sub> / HF | SiO <sub>2</sub>  | 125 mL | MSSI-100PPM  |
| Silver, Ag   | HNO <sub>3</sub>                         | Ag metal  | 125 mL | MSAG-100PPM  |
| Sodium, Na   | HNO <sub>3</sub>                         | Na <sub>2</sub> CO <sub>3</sub>   | 125 mL | MSNA-100PPM  |
| Strontium, Sr  | HNO <sub>3</sub>                         | SrCO <sub>3</sub>   | 125 mL | MSSR-100PPM  |
| Sulfur, S  | H <sub>2</sub> O                         | H <sub>2</sub> SO <sub>4</sub>  | 125 mL | MSS-100PPM   |
| Tellurium, Te  | HNO <sub>3</sub>                         | Te metal  | 125 mL | MSTEN-100PPM |
| Terbium, Tb  | HNO <sub>3</sub>                         | Tb <sub>4</sub> O <sub>7</sub>  | 125 mL | MSTB-100PPM  |
| Thallium, Tl   | HNO <sub>3</sub>                         | TlNO <sub>3</sub>   | 125 mL | MSTL-100PPM  |
| Thorium, Th  | HNO <sub>3</sub>                         | Th(NO <sub>3</sub> ) <sub>4</sub> ·xH <sub>2</sub> O                          | 125 mL | MSTH-100PPM  |
| Tin, Sn  | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Sn metal  | 125 mL | MSSN-100PPM  |
| Titanium, Ti   | HNO <sub>3</sub> / HF                    | Ti metal  | 125 mL | MSTI-100PPM  |
| Tungsten, W  | HNO <sub>3</sub> / HF                    | W Metal   | 125 mL | MSW-100PPM   |
| Uranium, U   | HNO <sub>3</sub>                         | UO <sub>2</sub> (NO <sub>3</sub> ) <sub>2</sub>                               | 125 mL | MSU-100PPM   |
| Vanadium, V  | HNO <sub>3</sub>                         | V <sub>2</sub> O <sub>5</sub>   | 125 mL | MSV-100PPM   |
| Yttrium, Y   | HNO <sub>3</sub>                         | Y <sub>2</sub> O <sub>3</sub>   | 125 mL | MSY-100PPM   |
| Zinc, Zn   | HNO <sub>3</sub>                         | Zn metal  | 125 mL | MSZN-100PPM  |

## 1000 µg/mL Standards

Custom 1000 µg/mL standards are available upon request.

1000 µg/mL

| Analyte   | Matrix                           | Starting Material   | Volume | Catalog # |
|---|----------------------------------|---|--------|-----------|
| Aluminum, Al  | HNO <sub>3</sub>                 | Al metal  | 125 mL | CGAL1-1   |
|   |                                  |   | 500 mL | CGAL1-5   |
| Aluminum, Al  | HCl                              | Al metal  | 125 mL | CGALCL1-1 |
|   |                                  |   | 500 mL | CGALCL1-5 |
| Antimony, Sb  | HNO <sub>3</sub> / Tartaric Acid | Sb metal  | 125 mL | CGSB1-1   |
|   |                                  |   | 500 mL | CGSB1-5   |
| Antimony, Sb  | HNO <sub>3</sub> / HF            | Sb metal  | 125 mL | CGSBF1-1  |
|   |                                  |   | 500 mL | CGSBF1-5  |
| Arsenic, As   | HNO <sub>3</sub>                 | As metal  | 125 mL | CGAS1-1   |
|   |                                  |   | 500 mL | CGAS1-5   |
| Barium, Ba  | HNO <sub>3</sub>                 | Ba(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | CGBA1-1   |
|   |                                  |   | 500 mL | CGBA1-5   |
| Beryllium, Be   | HNO <sub>3</sub>                 | Be <sub>4</sub> O(C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> ) <sub>6</sub> | 125 mL | CGBE1-1   |
|   |                                  |   | 500 mL | CGBE1-5   |
| Bismuth, Bi<br><small>Can be used as an Internal Standard for ICP-MS.</small>             | HNO <sub>3</sub>                 | Bi metal  | 125 mL | CGBI1-1   |
|   |                                  |   | 500 mL | CGBI1-5   |
| Boron, B  | H <sub>2</sub> O                 | H <sub>3</sub> BO <sub>3</sub>  | 125 mL | CGB1-1    |
|   |                                  |   | 500 mL | CGB1-5    |
| Bromide, Br <sup>-</sup><br><small>To be used for analyzing Bromide by ICP-OES.</small>   | H <sub>2</sub> O                 | NH <sub>4</sub> Br  | 125 mL | CGICBR1-1 |
|   |                                  |   | 500 mL | CGICBR1-5 |
| Cadmium, Cd   | HNO <sub>3</sub>                 | Cd metal  | 125 mL | CGCD1-1   |
|   |                                  |   | 500 mL | CGCD1-5   |
| Calcium, Ca   | HNO <sub>3</sub>                 | CaO   | 125 mL | CGCA1-1   |
|   |                                  |   | 500 mL | CGCA1-5   |
| Carbon, C   | HNO <sub>3</sub>                 | Tartaric acid   | 125 mL | CGC1-1    |
|   |                                  |   | 500 mL | CGC1-5    |
| Cerium, Ce  | HNO <sub>3</sub>                 | CeO <sub>2</sub>  | 125 mL | CGCE1-1   |
|   |                                  |   | 500 mL | CGCE1-5   |
| Cesium, Cs  | HNO <sub>3</sub>                 | CsNO <sub>3</sub>   | 125 mL | CGCS1-1   |
|   |                                  |   | 500 mL | CGCS1-5   |
| Chloride, Cl <sup>-</sup><br><small>To be used for analyzing Chloride by ICP-OES.</small> | H <sub>2</sub> O                 | NH <sub>4</sub> Cl  | 125 mL | CGICCL1-1 |
|   |                                  |   | 500 mL | CGICCL1-5 |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup>   | HNO <sub>3</sub>                 | Cr metal  | 125 mL | CGCR31-1  |
|   |                                  |   | 500 mL | CGCR31-5  |
| Chromium <sup>+6</sup> , Cr <sup>+6</sup>   | H <sub>2</sub> O                 | (NH <sub>4</sub> ) <sub>2</sub> Cr <sub>2</sub> O <sub>7</sub>                | 125 mL | CGCR61-1  |
|   |                                  |   | 500 mL | CGCR61-5  |
| Cobalt, Co  | HNO <sub>3</sub>                 | Co metal  | 125 mL | CGCO1-1   |
|   |                                  |   | 500 mL | CGCO1-5   |
| Copper, Cu  | HNO <sub>3</sub>                 | Cu metal  | 125 mL | CGCU1-1   |
|   |                                  |   | 500 mL | CGCU1-5   |
| Dysprosium, Dy  | HNO <sub>3</sub>                 | Dy <sub>2</sub> O <sub>3</sub>  | 125 mL | CGDY1-1   |
|   |                                  |   | 500 mL | CGDY1-5   |
| Erbium, Er  | HNO <sub>3</sub>                 | Er <sub>2</sub> O <sub>3</sub>  | 125 mL | CGER1-1   |
|   |                                  |   | 500 mL | CGER1-5   |
| Europium, Eu  | HNO <sub>3</sub>                 | Eu <sub>2</sub> O <sub>3</sub>  | 125 mL | CGEU1-1   |
|   |                                  |   | 500 mL | CGEU1-5   |

**1000 µg/mL Standards** (continued)

Custom 1000 µg/mL standards are available upon request.

**1000 µg/mL**

| Analyte  | Matrix                                   | Starting Material                                | Volume           | Catalog #            |
|--|--|--|------------------|----------------------|
| <b>Gadolinium, Gd</b>  | HNO <sub>3</sub>                         | Gd <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGGD1-1<br>CGGD1-5   |
| <b>Gallium, Ga</b>   | HNO <sub>3</sub>                         | Ga metal   | 125 mL<br>500 mL | CGGA1-1<br>CGGA1-5   |
| <b>Germanium, Ge</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Ge metal   | 125 mL<br>500 mL | CGGE1-1<br>CGGE1-5   |
| <b>Gold, Au</b>  | HCl                                      | AuCl <sub>3</sub>                                | 125 mL<br>500 mL | CGAU1-1<br>CGAU1-5   |
| <b>Gold, Au</b>  | HNO <sub>3</sub>                         | AuCl <sub>3</sub>                                | 125 mL<br>500 mL | CGAUN1-1<br>CGAUN1-5 |
| <b>Hafnium, Hf</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | HfO <sub>2</sub>                                 | 125 mL<br>500 mL | CGHF1-1<br>CGHF1-5   |
| <b>Holmium, Ho</b><br><small>Can be used as an Internal Standard for ICP-MS.</small>                         | HNO <sub>3</sub>                         | Ho <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGHO1-1<br>CGHO1-5   |
| <b>Indium, In</b><br><small>Can be used as an Internal Standard for ICP-MS.</small>                          | HNO <sub>3</sub>                         | In metal   | 125 mL<br>500 mL | CGIN1-1<br>CGIN1-5   |
| <b>Iodide, I<sup>-</sup></b><br><small>Can be used for analyzing Iodide by ICP-OES.</small>                  | H <sub>2</sub> O / stabilizer            | NH <sub>4</sub> I                                | 125 mL<br>500 mL | ICI1-1<br>ICI1-5     |
| <b>Iridium, Ir</b>   | HCl                                      | IrCl <sub>3</sub>                                | 125 mL<br>500 mL | CGIR1-1<br>CGIR1-5   |
| <b>Iron, Fe</b>  | HNO <sub>3</sub>                         | Fe metal   | 125 mL<br>500 mL | CGFE1-1<br>CGFE1-5   |
| <b>Lanthanum, La</b>   | HNO <sub>3</sub>                         | La <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGLA1-1<br>CGLA1-5   |
| <b>Lead, Pb</b>  | HNO <sub>3</sub>                         | Pb(NO <sub>3</sub> ) <sub>2</sub>                | 125 mL<br>500 mL | CGPB1-1<br>CGPB1-5   |
| <b>Lithium, Li</b>   | HNO <sub>3</sub>                         | Li <sub>2</sub> CO <sub>3</sub>                  | 125 mL<br>500 mL | CGLI1-1<br>CGLI1-5   |
| <b><sup>6</sup>Lithium, <sup>6</sup>Li</b><br><small>Can be used as an Internal Standard for ICP-MS.</small> | HNO <sub>3</sub>                         | <sup>6</sup> Li metal                            | 125 mL<br>500 mL | CG6LI1-1<br>CG6LI1-5 |
| <b>Lutetium, Lu</b>  | HNO <sub>3</sub>                         | Lu <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGLU1-1<br>CGLU1-5   |
| <b>Magnesium, Mg</b>   | HNO <sub>3</sub>                         | Mg metal   | 125 mL<br>500 mL | CGMG1-1<br>CGMG1-5   |
| <b>Manganese, Mn</b>   | HNO <sub>3</sub>                         | Mn metal   | 125 mL<br>500 mL | CGMN1-1<br>CGMN1-5   |
| <b>Mercury, Hg</b>   | HNO <sub>3</sub>                         | Hg metal   | 125 mL<br>500 mL | CGHG1-1<br>CGHG1-5   |
| <b>Molybdenum, Mo</b>  | H <sub>2</sub> O / NH <sub>4</sub> OH    | (NH <sub>4</sub> ) <sub>2</sub> MoO <sub>4</sub> | 125 mL<br>500 mL | CGMO1-1<br>CGMO1-5   |
| <b>Neodymium, Nd</b>   | HNO <sub>3</sub>                         | Nd <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGND1-1<br>CGND1-5   |
| <b>Nickel, Ni</b>  | HNO <sub>3</sub>                         | Ni metal   | 125 mL<br>500 mL | CGNI1-1<br>CGNI1-5   |
| <b>Niobium, Nb</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Nb metal   | 125 mL<br>500 mL | CGNB1-1<br>CGNB1-5   |

**1000 µg/mL Standards** (continued)

Custom 1000 µg/mL standards are available upon request.

1000 µg/mL

| Analyte                                       | Matrix                                   | Starting Material                                 | Volume           | Catalog #                |
|---|--|---|------------------|--------------------------|
| <b>Osmium, Os</b>                             | HCl                                      | (NH <sub>4</sub> ) <sub>2</sub> OsCl <sub>6</sub> | 125 mL           | CGOS1-1                  |
|   |  |   | 500 mL           | CGOS1-5                  |
| <b>Palladium, Pd</b>                          | HNO <sub>3</sub>                         | Pd(NO <sub>3</sub> ) <sub>2</sub>                 | 125 mL           | CGPDN1-1                 |
|   |  |   | 500 mL           | CGPDN1-5                 |
| <b>Palladium, Pd</b>                          | HCl                                      | Pd(NO <sub>3</sub> ) <sub>2</sub>                 | 125 mL<br>500 mL | CGPD1-1<br>CGPD1-5       |
| <b>Phosphorus, P</b>                          | H <sub>2</sub> O                         | H <sub>3</sub> PO <sub>4</sub>                    | 125 mL<br>500 mL | CGP1-1<br>CGP1-5         |
| <b>Platinum, Pt</b>                           | HNO <sub>3</sub> / HCl                   | Pt metal  | 125 mL           | CGPTN1-1                 |
|   |  |   | 500 mL           | CGPTN1-5                 |
| <b>Platinum, Pt</b>                           | HCl                                      | Pt metal  | 125 mL<br>500 mL | CGPT1-1<br>CGPT1-5       |
| <b>Potassium, K</b>                           | HNO <sub>3</sub>                         | KNO <sub>3</sub>                                  | 125 mL<br>500 mL | CGK1-1<br>CGK1-5         |
| <b>Praseodymium, Pr</b>                       | HNO <sub>3</sub>                         | Pr <sub>6</sub> O <sub>11</sub>                   | 125 mL<br>500 mL | CGPR1-1<br>CGPR1-5       |
| <b>Rhenium, Re</b>                            | HNO <sub>3</sub>                         | Re metal  | 125 mL<br>500 mL | CGRE1-1<br>CGRE1-5       |
| <b>Rhodium, Rh</b>                            | HCl                                      | RhCl <sub>3</sub>                                 | 125 mL<br>500 mL | CGRH1-1<br>CGRH1-5       |
| <b>Rhodium, Rh</b>                            | HNO <sub>3</sub>                         | RhNO <sub>3</sub>                                 | 125 mL<br>500 mL | CGRHN1-1<br>CGRHN1-5     |
| <b>Rubidium, Rb</b>                           | HNO <sub>3</sub>                         | RbNO <sub>3</sub>                                 | 125 mL<br>500 mL | CGRB1-1<br>CGRB1-5       |
| <b>Ruthenium, Ru</b>                          | HCl                                      | NH <sub>4</sub> RuCl <sub>6</sub>                 | 125 mL<br>500 mL | CGRU1-1<br>CGRU1-5       |
| <b>Samarium, Sm</b>                           | HNO <sub>3</sub>                         | Sm <sub>2</sub> O <sub>3</sub>                    | 125 mL<br>500 mL | CGSM1-1<br>CGSM1-5       |
| <b>Scandium, Sc</b>                           | HNO <sub>3</sub>                         | Sc <sub>2</sub> O <sub>3</sub>                    | 125 mL<br>500 mL | CGSC1-1<br>CGSC1-5       |
| <b>Selenium<sup>+4</sup>, Se<sup>+4</sup></b> | HNO <sub>3</sub>                         | Se metal  | 125 mL<br>500 mL | CGSE41-1<br>CGSE41-5     |
| <b>Silica, SiO<sub>2</sub></b>                | HNO <sub>3</sub> / HF                    | SiO <sub>2</sub>                                  | 125 mL           | CGSIO1-1                 |
|   |  |   | 500 mL           | CGSIO1-5                 |
| <b>Silica, SiO<sub>2</sub></b>                | NaOH                                     | SiO <sub>2</sub>                                  | 125 mL<br>500 mL | CGSIONA1-1<br>CGSIONA1-5 |
| <b>Silicon, Si</b>                            | H <sub>2</sub> O / HNO <sub>3</sub> / HF | SiO <sub>2</sub>                                  | 125 mL<br>500 mL | CGSI1-1<br>CGSI1-5       |
| <b>Silicon, Si</b>                            | NaOH                                     | SiO <sub>2</sub>                                  | 125 mL<br>500 mL | CGSINA1-1<br>CGSINA1-5   |
| <b>Silver, Ag</b>                             | HNO <sub>3</sub>                         | Ag metal  | 125 mL<br>500 mL | CGAG1-1<br>CGAG1-5       |
| <b>Sodium, Na</b>                             | HNO <sub>3</sub>                         | Na <sub>2</sub> CO <sub>3</sub>                   | 125 mL<br>500 mL | CGNA1-1<br>CGNA1-5       |
| <b>Strontium, Sr</b>                          | HNO <sub>3</sub>                         | SrCO <sub>3</sub>                                 | 125 mL<br>500 mL | CGSR1-1<br>CGSR1-5       |
| <b>Sulfur, S</b>                              | H <sub>2</sub> O                         | Methanesulfonic acid                              | 125 mL           | CGMSA1-1                 |
|   |  |   | 500 mL           | CGMSA1-5                 |

**NEW**

Can be used as an Internal Standard for ICP-MS.

Can be used as an Internal Standard for ICP-MS.

Can be used as an Internal Standard for ICP-MS.

Prevents incompatibility issues when mixing with Ba and Pb.

**1000 µg/mL Standards** (continued)

Custom 1000 µg/mL standards are available upon request.

**1000 µg/mL**

| Analyte  | Matrix                                   | Starting Material                                    | Volume           | Catalog #              |
|--|--|--|------------------|------------------------|
| <b>Sulfur, S</b>   | H <sub>2</sub> O                         | H <sub>2</sub> SO <sub>4</sub>                       | 125 mL<br>500 mL | CGS1-1<br>CGS1-5       |
| <b>Tantalum, Ta</b>  | HNO <sub>3</sub> / HF                    | Ta metal   | 125 mL<br>500 mL | CGTA1-1<br>CGTA1-5     |
| <b>Tellurium, Te</b>   | HCl                                      | Te metal   | 125 mL<br>500 mL | CGTE1-1<br>CGTE1-5     |
| <b>Tellurium, Te</b>   | HNO <sub>3</sub>                         | Te metal   | 125 mL<br>500 mL | CGTEN1-1<br>CGTEN1-5   |
| <b>Terbium, Tb</b><br><small>Can be used as an Internal Standard for ICP-MS.</small> | HNO <sub>3</sub>                         | Tb <sub>4</sub> O <sub>7</sub>                       | 125 mL<br>500 mL | CGTB1-1<br>CGTB1-5     |
| <b>Thallium, Tl</b>  | HNO <sub>3</sub>                         | TlNO <sub>3</sub>                                    | 125 mL<br>500 mL | CGTL1-1<br>CGTL1-5     |
| <b>Thorium, Th</b>   | HNO <sub>3</sub>                         | Th(NO <sub>3</sub> ) <sub>4</sub> ·xH <sub>2</sub> O | 125 mL<br>500 mL | CGTH1-1<br>CGTH1-5     |
| <b>Thulium, Tm</b>   | HNO <sub>3</sub>                         | Tm <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGTM1-1<br>CGTM1-5     |
| <b>Tin, Sn</b>   | HCl                                      | Sn metal   | 125 mL<br>500 mL | CGSNCL1-1<br>CGSNCL1-5 |
| <b>Tin, Sn</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Sn metal   | 125 mL<br>500 mL | CGSN1-1<br>CGSN1-5     |
| <b>Titanium, Ti</b>  | HNO <sub>3</sub> / HF                    | Ti metal   | 125 mL<br>500 mL | CGTI1-1<br>CGTI1-5     |
| <b>Tungsten, W</b>   | HNO <sub>3</sub> / HF                    | W metal  | 125 mL<br>500 mL | CGW1-1<br>CGW1-5       |
| <b>Uranium, U</b>  | HNO <sub>3</sub>                         | UO <sub>2</sub> (NO <sub>3</sub> ) <sub>2</sub>      | 125 mL<br>500 mL | CGU1-1<br>CGU1-5       |
| <b>Vanadium, V</b>   | HNO <sub>3</sub>                         | V <sub>2</sub> O <sub>5</sub>                        | 125 mL<br>500 mL | CGV1-1<br>CGV1-5       |
| <b>Ytterbium, Yb</b>   | HNO <sub>3</sub>                         | Yb <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGYB1-1<br>CGYB1-5     |
| <b>Yttrium, Y</b><br><small>Can be used as an Internal Standard for ICP-MS.</small>  | HNO <sub>3</sub>                         | Y <sub>2</sub> O <sub>3</sub>                        | 125 mL<br>500 mL | CGY1-1<br>CGY1-5       |
| <b>Zinc, Zn</b>  | HNO <sub>3</sub>                         | Zn metal   | 125 mL<br>500 mL | CGZN1-1<br>CGZN1-5     |
| <b>Zirconium, Zr</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | ZrO <sub>2</sub>                                     | 125 mL<br>500 mL | CGZR1-1<br>CGZR1-5     |

**Exceptional...**

The quality of Inorganic Ventures' service is exceptional. There's always a live person when you call and I always get a response to every inquiry. With their level of quality in products and service, they've become the "standards" industry.

*Sally Gemora  
Hayward, CA*

**10,000 µg/mL Standards**

Custom 10,000 µg/mL standards are available upon request.

**10,000 µg/mL**

| Analyte   | Matrix                                   | Starting Material   | Volume           | Catalog #              |
|---|--|---|------------------|------------------------|
| <b>Aluminum, Al</b>   | HNO <sub>3</sub>                         | Al metal  | 125 mL<br>500 mL | CGAL10-1<br>CGAL10-5   |
| <b>Antimony, Sb</b>   | HNO <sub>3</sub> / Tartaric Acid         | Sb metal  | 125 mL<br>500 mL | CGSB10-1<br>CGSB10-5   |
| <b>Arsenic, As</b>  | HNO <sub>3</sub>                         | As metal  | 125 mL<br>500 mL | CGAS10-1<br>CGAS10-5   |
| <b>Barium, Ba</b>   | HNO <sub>3</sub>                         | Ba(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL<br>500 mL | CGBA10-1<br>CGBA10-5   |
| <b>Beryllium, Be</b>  | HNO <sub>3</sub>                         | Be <sub>4</sub> O(C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> ) <sub>6</sub> | 125 mL<br>500 mL | CGBE10-1<br>CGBE10-5   |
| <b>Bismuth, Bi</b>  | HNO <sub>3</sub>                         | Bi metal  | 125 mL<br>500 mL | CGBI10-1<br>CGBI10-5   |
| <b>Boron, B</b>   | NH <sub>4</sub> OH                       | H <sub>3</sub> BO <sub>3</sub>  | 125 mL<br>500 mL | CGB10-1<br>CGB10-5     |
| <b>Cadmium, Cd</b>  | HNO <sub>3</sub>                         | Cd metal  | 125 mL<br>500 mL | CGCD10-1<br>CGCD10-5   |
| <b>Calcium, Ca</b>  | HNO <sub>3</sub>                         | CaO   | 125 mL<br>500 mL | CGCA10-1<br>CGCA10-5   |
| <b>Carbon, C</b>  | HNO <sub>3</sub>                         | Tartaric acid   | 125 mL<br>500 mL | CGC10-1<br>CGC10-5     |
| <b>Cerium, Ce</b>   | HNO <sub>3</sub>                         | CeO <sub>2</sub>  | 125 mL<br>500 mL | CGCE10-1<br>CGCE10-5   |
| <b>Cesium, Cs</b>   | HNO <sub>3</sub>                         | CsNO <sub>3</sub>   | 125 mL<br>500 mL | CGCS10-1<br>CGCS10-5   |
| <b>Chromium<sup>+3</sup>, Cr<sup>+3</sup></b>                                       | HNO <sub>3</sub>                         | Cr metal  | 125 mL<br>500 mL | CGCR310-1<br>CGCR310-5 |
| <b>Cobalt, Co</b><br><small>Can be used as an Internal Standard for ICP-OES</small> | HNO <sub>3</sub>                         | Co metal  | 125 mL<br>500 mL | CGCO10-1<br>CGCO10-5   |
| <b>Copper, Cu</b>   | HNO <sub>3</sub>                         | Cu metal  | 125 mL<br>500 mL | CGCU10-1<br>CGCU10-5   |
| <b>Dysprosium, Dy</b>   | HNO <sub>3</sub>                         | Dy <sub>2</sub> O <sub>3</sub>  | 125 mL<br>500 mL | CGDY10-1<br>CGDY10-5   |
| <b>Erbium, Er</b>   | HNO <sub>3</sub>                         | Er <sub>2</sub> O <sub>3</sub>  | 125 mL<br>500 mL | CGER10-1<br>CGER10-5   |
| <b>Europium, Eu</b>   | HNO <sub>3</sub>                         | Eu <sub>2</sub> O <sub>3</sub>  | 125 mL<br>500 mL | CGEU10-1<br>CGEU10-5   |
| <b>Gadolinium, Gd</b>   | HNO <sub>3</sub>                         | Gd <sub>2</sub> O <sub>3</sub>  | 125 mL<br>500 mL | CGGD10-1<br>CGGD10-5   |
| <b>Gallium, Ga</b>  | HNO <sub>3</sub>                         | Ga metal  | 125 mL<br>500 mL | CGGA10-1<br>CGGA10-5   |
| <b>Germanium, Ge</b>  | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Ge metal  | 125 mL<br>500 mL | CGGE10-1<br>CGGE10-5   |
| <b>Gold, Au</b>   | HCl                                      | AuCl <sub>3</sub>   | 125 mL<br>500 mL | CGAU10-1<br>CGAU10-5   |
| <b>Hafnium, Hf</b>  | HNO <sub>3</sub> / HF                    | HfO <sub>2</sub>  | 125 mL<br>500 mL | CGHF10-1<br>CGHF10-5   |
| <b>Holmium, Ho</b>  | HNO <sub>3</sub>                         | Ho <sub>2</sub> O <sub>3</sub>  | 125 mL<br>500 mL | CGHO10-1<br>CGHO10-5   |

**10,000 µg/mL Standards** (continued)

Custom 10,000 µg/mL standards are available upon request.

**10,000 µg/mL**

| Analyte  | Matrix                                   | Starting Material                                | Volume           | Catalog #            |
|--|--|--|------------------|----------------------|
| <b>Indium, In</b>                                | HNO <sub>3</sub>                         | In metal   | 125 mL<br>500 mL | CGIN10-1<br>CGIN10-5 |
| Can be used as an Internal Standard for ICP-OES. |  |  |                  |                      |
| <b>Iridium, Ir</b>                               | HCl                                      | IrCl <sub>3</sub>                                | 125 mL<br>500 mL | CGIR10-1<br>CGIR10-5 |
| <b>Iron, Fe</b>                                  | HNO <sub>3</sub>                         | Fe metal   | 125 mL<br>500 mL | CGFE10-1<br>CGFE10-5 |
| <b>Lanthanum, La</b>                             | HNO <sub>3</sub>                         | La <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGLA10-1<br>CGLA10-5 |
| <b>Lead, Pb</b>                                  | HNO <sub>3</sub>                         | Pb(NO <sub>3</sub> ) <sub>2</sub>                | 125 mL<br>500 mL | CGPB10-1<br>CGPB10-5 |
| <b>Lithium, Li</b>                               | HNO <sub>3</sub>                         | Li <sub>2</sub> CO <sub>3</sub>                  | 125 mL<br>500 mL | CGLI10-1<br>CGLI10-5 |
| <b>Lutetium, Lu</b>                              | HNO <sub>3</sub>                         | Lu <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGLU10-1<br>CGLU10-5 |
| <b>Magnesium, Mg</b>                             | HNO <sub>3</sub>                         | Mg metal   | 125 mL<br>500 mL | CGMG10-1<br>CGMG10-5 |
| <b>Manganese, Mn</b>                             | HNO <sub>3</sub>                         | Mn metal   | 125 mL<br>500 mL | CGMN10-1<br>CGMN10-5 |
| <b>Mercury, Hg</b>                               | HNO <sub>3</sub>                         | Hg metal   | 125 mL<br>500 mL | CGHG10-1<br>CGHG10-5 |
| <b>Molybdenum, Mo</b>                            | H <sub>2</sub> O / NH <sub>4</sub> OH    | (NH <sub>4</sub> ) <sub>2</sub> MoO <sub>4</sub> | 125 mL<br>500 mL | CGMO10-1<br>CGMO10-5 |
| <b>Neodymium, Nd</b>                             | HNO <sub>3</sub>                         | Nd <sub>2</sub> O <sub>3</sub>                   | 125 mL<br>500 mL | CGND10-1<br>CGND10-5 |
| <b>Nickel, Ni</b>                                | HNO <sub>3</sub>                         | Ni metal   | 125 mL<br>500 mL | CGNI10-1<br>CGNI10-5 |
| <b>Niobium, Nb</b>                               | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Nb metal   | 125 mL<br>500 mL | CGNB10-1<br>CGNB10-5 |
| <b>Palladium, Pd</b>                             | HCl                                      | Pd(NO <sub>3</sub> ) <sub>2</sub>                | 125 mL<br>500 mL | CGPD10-1<br>CGPD10-5 |
| <b>Phosphorus, P</b>                             | H <sub>2</sub> O                         | H <sub>3</sub> PO <sub>4</sub>                   | 125 mL<br>500 mL | CGP10-1<br>CGP10-5   |
| <b>Platinum, Pt</b>                              | HCl                                      | Pt metal   | 125 mL<br>500 mL | CGPT10-1<br>CGPT10-5 |
| <b>Potassium, K</b>                              | HNO <sub>3</sub>                         | KNO <sub>3</sub>                                 | 125 mL<br>500 mL | CGK10-1<br>CGK10-5   |
| <b>Praseodymium, Pr</b>                          | HNO <sub>3</sub>                         | Pr <sub>6</sub> O <sub>11</sub>                  | 125 mL<br>500 mL | CGPR10-1<br>CGPR10-5 |
| <b>Rhenium, Re</b>                               | HNO <sub>3</sub>                         | Re metal   | 125 mL<br>500 mL | CGRE10-1<br>CGRE10-5 |
| <b>Rhodium, Rh</b>                               | HCl                                      | RhCl <sub>3</sub>                                | 125 mL<br>500 mL | CGRH10-1<br>CGRH10-5 |
| <b>Rubidium, Rb</b>                              | HNO <sub>3</sub>                         | RbNO <sub>3</sub>                                | 125 mL<br>500 mL | CGRB10-1<br>CGRB10-5 |
| <b>Ruthenium, Ru</b>                             | HCl                                      | NH <sub>4</sub> RuCl <sub>6</sub>                | 125 mL<br>500 mL | CGRU10-1<br>CGRU10-5 |

**10,000 µg/mL Standards** (continued)

Custom 10,000 µg/mL standards are available upon request.

**10,000 µg/mL**

| Analyte  | Matrix                                   | Starting Material                                    | Volume           | Catalog #              |
|--|--|--|------------------|------------------------|
| <b>Samarium, Sm</b>  | HNO <sub>3</sub>                         | Sm <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGSM10-1<br>CGSM10-5   |
| <b>Scandium, Sc</b>  | HNO <sub>3</sub>                         | Sc <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGSC10-1<br>CGSC10-5   |
| <small>Can be used as an Internal Standard for ICP-OES.</small>            |  |  |                  |                        |
| <b>Selenium, Se</b>  | HNO <sub>3</sub>                         | Se metal   | 125 mL<br>500 mL | CGSE10-1<br>CGSE10-5   |
| <b>Silicon, Si</b>   | HNO <sub>3</sub> / HF                    | SiO <sub>2</sub>                                     | 125 mL<br>500 mL | CGSI10-1<br>CGSI10-5   |
| <b>Silver, Ag</b>  | HNO <sub>3</sub>                         | Ag metal   | 125 mL<br>500 mL | CGAG10-1<br>CGAG10-5   |
| <b>Sodium, Na</b>  | HNO <sub>3</sub>                         | Na <sub>2</sub> CO <sub>3</sub>                      | 125 mL<br>500 mL | CGNA10-1<br>CGNA10-5   |
| <b>Strontium, Sr</b>   | HNO <sub>3</sub>                         | SrCO <sub>3</sub>                                    | 125 mL<br>500 mL | CGSR10-1<br>CGSR10-5   |
| <b>Sulfur, S</b>   | H <sub>2</sub> O                         | Methanesulfonic acid                                 | 125 mL<br>500 mL | CGMSA10-1<br>CGMSA10-5 |
| <small>Prevents incompatibility issues when mixing with Ba and Pb.</small> |  |  |                  |                        |
| <b>Sulfur, S</b>   | H <sub>2</sub> O                         | H <sub>2</sub> SO <sub>4</sub>                       | 125 mL<br>500 mL | CGS10-1<br>CGS10-5     |
| <b>Tantalum, Ta</b>  | HNO <sub>3</sub> / HF                    | Ta metal   | 125 mL<br>500 mL | CGTA10-1<br>CGTA10-5   |
| <b>Tellurium, Te</b>   | HCl                                      | Te metal   | 125 mL<br>500 mL | CGTE10-1<br>CGTE10-5   |
| <b>Terbium, Tb</b>   | HNO <sub>3</sub>                         | Tb <sub>4</sub> O <sub>7</sub>                       | 125 mL<br>500 mL | CGTB10-1<br>CGTB10-5   |
| <b>Thallium, Tl</b>  | HNO <sub>3</sub>                         | TlNO <sub>3</sub>                                    | 125 mL<br>500 mL | CGTL10-1<br>CGTL10-5   |
| <b>Thorium, Th</b>   | HNO <sub>3</sub>                         | Th(NO <sub>3</sub> ) <sub>4</sub> ·xH <sub>2</sub> O | 125 mL<br>500 mL | CGTH10-1<br>CGTH10-5   |
| <b>Thulium, Tm</b>   | HNO <sub>3</sub>                         | Tm <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGTM10-1<br>CGTM10-5   |
| <b>Tin, Sn</b>   | H <sub>2</sub> O / HNO <sub>3</sub> / HF | Sn metal   | 125 mL<br>500 mL | CGSN10-1<br>CGSN10-5   |
| <b>Titanium, Ti</b>  | HNO <sub>3</sub> / HF                    | Ti metal   | 125 mL<br>500 mL | CGTI10-1<br>CGTI10-5   |
| <b>Tungsten, W</b>   | HNO <sub>3</sub> / HF                    | W metal  | 125 mL<br>500 mL | CGW10-1<br>CGW10-5     |
| <b>Uranium, U</b>  | HNO <sub>3</sub>                         | UO <sub>2</sub> (NO <sub>3</sub> ) <sub>2</sub>      | 125 mL<br>500 mL | CGU10-1<br>CGU10-5     |
| <b>Vanadium, V</b>   | HNO <sub>3</sub>                         | V <sub>2</sub> O <sub>5</sub>                        | 125 mL<br>500 mL | CGV10-1<br>CGV10-5     |
| <b>Ytterbium, Yb</b>   | HNO <sub>3</sub>                         | Yb <sub>2</sub> O <sub>3</sub>                       | 125 mL<br>500 mL | CGYB10-1<br>CGYB10-5   |
| <b>Yttrium, Y</b>  | HNO <sub>3</sub>                         | Y <sub>2</sub> O <sub>3</sub>                        | 125 mL<br>500 mL | CGY10-1<br>CGY10-5     |
| <small>Can be used as an Internal Standard for ICP-OES.</small>            |  |  |                  |                        |
| <b>Zinc, Zn</b>  | HNO <sub>3</sub>                         | Zn metal   | 125 mL<br>500 mL | CGZN10-1<br>CGZN10-5   |
| <b>Zirconium, Zr</b>   | HF                                       | ZrO <sub>2</sub>                                     | 125 mL<br>500 mL | CGZR10-1<br>CGZR10-5   |

NEW

NEW

Custom isotopic standards are available upon request.

| Analyte  | ug/mL | Matrix                | Starting Material                | Volume           | Catalog #            |
|--|-------|-----------------------|----------------------------------|------------------|----------------------|
| <sup>135</sup> Barium, <sup>135</sup> Ba                       | 10    | HNO <sub>3</sub>      | <sup>135</sup> BaCO <sub>3</sub> | 100 mL           | MS135BA-10PPM        |
| <sup>10</sup> Boron, <sup>10</sup> B                           | 10    | NH <sub>4</sub> OH    | <sup>10</sup> B oxide            | 100 mL           | MS10B-10PPM          |
| <sup>11</sup> Boron, <sup>11</sup> B                           | 10    | NH <sub>4</sub> OH    | <sup>11</sup> B oxide            | 100 mL           | MS11B-10PPM          |
| <sup>106</sup> Cadmium, <sup>106</sup> Cd                      | 10    | HNO <sub>3</sub>      | <sup>106</sup> Cd metal          | 100 mL           | MS106CD-10PPM        |
| <sup>50</sup> Chromium, <sup>50</sup> Cr                       | 10    | HNO <sub>3</sub>      | <sup>50</sup> Cr metal           | 100 mL           | MS50CR-10PPM         |
| <sup>65</sup> Copper, <sup>65</sup> Cu                         | 10    | HNO <sub>3</sub>      | <sup>65</sup> Cu metal           | 100 mL           | MS65CU-10PPM         |
| <sup>54</sup> Iron, <sup>54</sup> Fe                           | 10    | HNO <sub>3</sub>      | <sup>54</sup> Fe metal           | 100 mL           | MS54FE-10PPM         |
| <sup>57</sup> Iron, <sup>57</sup> Fe                           | 10    | HNO <sub>3</sub>      | <sup>57</sup> Fe metal           | 100 mL           | MS57FE-10PPM         |
| <sup>204</sup> Lead, <sup>204</sup> Pb                         | 10    | HNO <sub>3</sub>      | <sup>204</sup> PbCO <sub>3</sub> | 100 mL           | MS204PB-10PPM        |
| <sup>206</sup> Lead, <sup>206</sup> Pb                         | 10    | HNO <sub>3</sub>      | <sup>206</sup> PbCO <sub>3</sub> | 100 mL           | MS206PB-10PPM        |
| <sup>207</sup> Lead, <sup>207</sup> Pb                         | 10    | HNO <sub>3</sub>      | <sup>207</sup> PbCO <sub>3</sub> | 100 mL           | MS207PB-10PPM        |
| <sup>6</sup> Lithium, <sup>6</sup> Li                          | 10    | HNO <sub>3</sub>      | <sup>6</sup> Li metal            | 125 mL           | MS6LI-10PPM          |
| <sup>6</sup> Lithium, <sup>6</sup> Li                          | 100   | HNO <sub>3</sub>      | <sup>6</sup> Li metal            | 125 mL           | MS6LI-100PPM         |
| <sup>6</sup> Lithium, <sup>6</sup> Li                          | 1000  | HNO <sub>3</sub>      | <sup>6</sup> Li metal            | 125 mL<br>500 mL | CG6LI1-1<br>CG6LI1-5 |
| <small>Can be used as an Internal Standard for ICP-MS.</small> |       |                       |                                  |                  |                      |
| <sup>25</sup> Magnesium, <sup>25</sup> Mg                      | 10    | HNO <sub>3</sub>      | <sup>25</sup> MgO                | 100 mL           | MS25MG-10PPM         |
| <sup>61</sup> Nickel, <sup>61</sup> Ni                         | 10    | HNO <sub>3</sub>      | <sup>61</sup> Ni metal           | 100 mL           | MS61NI-10PPM         |
| <sup>78</sup> Selenium, <sup>78</sup> Se                       | 10    | HNO <sub>3</sub>      | <sup>78</sup> Se metal           | 100 mL           | MS78SE-10PPM         |
| <sup>82</sup> Selenium, <sup>82</sup> Se                       | 10    | HNO <sub>3</sub>      | <sup>82</sup> Se metal           | 100 mL           | MS82SE-10PPM         |
| <sup>109</sup> Silver, <sup>109</sup> Ag                       | 10    | HNO <sub>3</sub>      | <sup>109</sup> Ag metal          | 100 mL           | MS109AG-10PPM        |
| <sup>86</sup> Strontium, <sup>86</sup> Sr                      | 10    | HNO <sub>3</sub>      | <sup>86</sup> SrCO <sub>3</sub>  | 100 mL           | MS86SR-10PPM         |
| <sup>203</sup> Thallium, <sup>203</sup> Tl                     | 10    | HNO <sub>3</sub>      | <sup>203</sup> Tl oxide          | 100 mL           | MS203TL-10PPM        |
| <sup>205</sup> Thallium, <sup>205</sup> Tl                     | 10    | HNO <sub>3</sub>      | <sup>205</sup> Tl oxide          | 100 mL           | MS205TL-10PPM        |
| <sup>122</sup> Tin, <sup>122</sup> Sn                          | 10    | HNO <sub>3</sub> / HF | <sup>122</sup> Sn metal          | 100 mL           | MS122SN-10PPM        |
| <sup>67</sup> Zinc, <sup>67</sup> Zn                           | 10    | HNO <sub>3</sub>      | <sup>67</sup> Zn metal           | 100 mL           | MS67ZN-10PPM         |

*"In the lab, our primary goal is to produce accurate and dependable standards. Everything we make is backed by our 100% Satisfaction Guarantee."*

**Jenna Case**  
Manufacturing Technician



## SPECIATION STANDARDS

Custom speciation standards are available upon request.

| Analyte                                   | ug/mL  | Matrix                              | Starting Material  | Volume           | Catalog #              |
|---|--------|-------------------------------------|--|------------------|------------------------|
| Arsenic <sup>+3</sup> , As <sup>+3</sup>  | 1000   | HCl / NaOH /<br>NaHCO <sub>3</sub>  | As <sub>2</sub> O <sub>3</sub>                                 | 125 mL<br>500 mL | CGAS31-1<br>CGAS31-5   |
| Arsenic <sup>+5</sup> , As <sup>+5</sup>  | 1000   | H <sub>2</sub> O                    | As <sub>2</sub> O <sub>5</sub>                                 | 125 mL<br>500 mL | CGAS51-1<br>CGAS51-5   |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup> | 10     | HNO <sub>3</sub>                    | Cr metal   | 125 mL           | MSCR3-10PPM            |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup> | 100    | HNO <sub>3</sub>                    | Cr metal   | 125 mL           | MSCR3-100PPM           |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup> | 1000   | HNO <sub>3</sub>                    | Cr metal   | 125 mL<br>500 mL | CGCR31-1<br>CGCR31-5   |
| Chromium <sup>+3</sup> , Cr <sup>+3</sup> | 10,000 | HNO <sub>3</sub>                    | Cr metal   | 125 mL<br>500 mL | CGCR310-1<br>CGCR310-5 |
| Chromium <sup>+6</sup> , Cr <sup>+6</sup> | 1000   | H <sub>2</sub> O                    | (NH <sub>4</sub> ) <sub>2</sub> Cr <sub>2</sub> O <sub>7</sub> | 125 mL<br>500 mL | CGCR61-1<br>CGCR61-5   |
| Selenium <sup>+4</sup> , Se <sup>+4</sup> | 1000   | HNO <sub>3</sub>                    | Se metal   | 125 mL<br>500 mL | CGSE41-1<br>CGSE41-5   |
| Selenium <sup>+6</sup> , Se <sup>+6</sup> | 1000   | H <sub>2</sub> O / HNO <sub>3</sub> | Selenic acid   | 125 mL<br>500 mL | CGSE61-1<br>CGSE61-5   |

## CYANIDE STANDARDS

## 1000 µg/mL Standards

Custom cyanide standards are available upon request.

| Analyte    | ug/mL | Matrix | Starting Material | Volume           | Catalog #            |
|------------|-------|--------|-------------------|------------------|----------------------|
| Copper, Cu | 1000  | NaCN   | Cu metal          | 125 mL<br>500 mL | AACUCN-1<br>AACUCN-5 |
| Gold, Au   | 1000  | NaCN   | AuCl <sub>3</sub> | 125 mL<br>500 mL | AAAUCN-1<br>AAAUCN-5 |
| Silver, Ag | 1000  | NaCN   | Ag metal          | 125 mL<br>500 mL | AAAGCN-1<br>AAAGCN-5 |
| Zinc, Zn   | 1000  | NaCN   | Zn metal          | 125 mL<br>500 mL | AAZNCN-1<br>AAZNCN-5 |

## Convenient...

In addition to utilizing your off-the-shelf standards for IC and AA, our laboratory also utilizes custom ICP-MS standards. Aside from your usual exceptional quality, you package these 250 mL volumes in two 125 mL packages for ultimate convenience and efficiency at no extra cost.

*Jo Holcomb  
Grand Junction, CO*

## Calibration Standards

These elements are grouped for ease of use. Intended for ICP-MS, they can be used individually or combined in any combination upon dilution into 1% HNO<sub>3</sub>. Custom calibration standards are available upon request.

### 65-Element Group

#### Rare Earth ICP-MS Standard

| CMS-1   |                  |         |       |
|---------|------------------|---------|-------|
| Volume  | 125 mL           |         |       |
| Matrix  | HNO <sub>3</sub> |         |       |
| Analyte | µg/mL            | Analyte | µg/mL |
| Ce      | 10               | Pr      | 10    |
| Dy      | 10               | Sc      | 10    |
| Er      | 10               | Sm      | 10    |
| Eu      | 10               | Tb      | 10    |
| Gd      | 10               | Th      | 10    |
| Ho      | 10               | Tm      | 10    |
| La      | 10               | U       | 10    |
| Lu      | 10               | Y       | 10    |
| Nd      | 10               | Yb      | 10    |

#### Precious Metals ICP-MS Standard

| CMS-2   |        |         |       |
|---------|--------|---------|-------|
| Volume  | 125 mL |         |       |
| Matrix  | HCl    |         |       |
| Analyte | µg/mL  | Analyte | µg/mL |
| Au      | 10     | Re      | 10    |
| Ir      | 10     | Rh      | 10    |
| Pd      | 10     | Ru      | 10    |
| Pt      | 10     | Te      | 10    |

#### Fluoride Soluble ICP-MS Standard

| CMS-3   |                       |         |       |
|---------|-----------------------|---------|-------|
| Volume  | 125 mL                |         |       |
| Matrix  | HNO <sub>3</sub> / HF |         |       |
| Analyte | µg/mL                 | Analyte | µg/mL |
| Ge      | 10                    | Ta      | 10    |
| Hf      | 10                    | Ti      | 10    |
| Mo      | 10                    | W       | 10    |
| Nb      | 10                    | Zr      | 10    |
| Sn      | 10                    |         |       |

#### Hot-Plasma ICP-MS Complete Standard

| CMS-4   |                  |         |       |
|---------|------------------|---------|-------|
| Volume  | 125 mL           |         |       |
| Matrix  | HNO <sub>3</sub> |         |       |
| Analyte | µg/mL            | Analyte | µg/mL |
| As      | 10               | In      | 10    |
| B       | 10               | Pb      | 10    |
| Ba      | 10               | Sb      | 10    |
| Be      | 10               | Se      | 10    |
| Bi      | 10               | Tl      | 10    |
| Cd      | 10               | V       | 10    |
| Ga      | 10               |         |       |

#### Cool-Plasma ICP-MS Complete Standard

| CMS-5   |                  |         |       |
|---------|------------------|---------|-------|
| Volume  | 125 mL           |         |       |
| Matrix  | HNO <sub>3</sub> |         |       |
| Analyte | µg/mL            | Analyte | µg/mL |
| Ag      | 10               | Li      | 10    |
| Al      | 10               | Mg      | 10    |
| Ca      | 10               | Mn      | 10    |
| Co      | 10               | Na      | 10    |
| Cr      | 10               | Ni      | 10    |
| Cs      | 10               | Rb      | 10    |
| Cu      | 10               | Sr      | 10    |
| Fe      | 10               | Zn      | 10    |
| K       | 10               |         |       |

### Educational...

We maintain a wide range of individual elements and a variety of custom standards made by Inorganic Ventures, which have all performed very well. Their website also contains a wealth of information, which continues to expand. The articles by Dr. Paul Gaines are very useful.

*Lynn Schurter  
Granville, OH*

**Calibration Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**69-Element Group****Rare Earths ICP-MS Standard**

|                |                  |                |              |
|----------------|------------------|----------------|--------------|
| CCS-1          |                  |                |              |
| Volume         | 125 mL           |                |              |
| Matrix         | HNO <sub>3</sub> |                |              |
| <b>Analyte</b> | <b>µg/mL</b>     | <b>Analyte</b> | <b>µg/mL</b> |
| Ce             | 100              | Pr             | 100          |
| Dy             | 100              | Sc             | 100          |
| Er             | 100              | Sm             | 100          |
| Eu             | 100              | Tb             | 100          |
| Gd             | 100              | Th             | 100          |
| Ho             | 100              | Tm             | 100          |
| La             | 100              | U              | 100          |
| Lu             | 100              | Y              | 100          |
| Nd             | 100              | Yb             | 100          |

**Precious Metals ICP-MS Standard**

|                |              |                |              |
|----------------|--------------|----------------|--------------|
| CCS-2          |              |                |              |
| Volume         | 125 mL       |                |              |
| Matrix         | HCl          |                |              |
| <b>Analyte</b> | <b>µg/mL</b> | <b>Analyte</b> | <b>µg/mL</b> |
| Au             | 100          | Pt             | 100          |
| Ir             | 100          | Rh             | 100          |
| Pd             | 100          | Ru             | 100          |

**Alkali, Alkaline, Non-Transition ICP-MS Standard**

|                |                  |                |              |
|----------------|------------------|----------------|--------------|
| CCS-4          |                  |                |              |
| Volume         | 125 mL           |                |              |
| Matrix         | HNO <sub>3</sub> |                |              |
| <b>Analyte</b> | <b>µg/mL</b>     | <b>Analyte</b> | <b>µg/mL</b> |
| Al             | 100              | In             | 100          |
| As             | 100              | K              | 100          |
| Ba             | 100              | Li             | 100          |
| Be             | 100              | Mg             | 100          |
| Bi             | 100              | Na             | 100          |
| Ca             | 100              | Rb             | 100          |
| Cs             | 100              | Se             | 100          |
| Ga             | 100              | Sr             | 100          |

**Fluoride Soluble ICP-MS Standard**

|                |                       |                |              |
|----------------|-----------------------|----------------|--------------|
| CCS-5          |                       |                |              |
| Volume         | 125 mL                |                |              |
| Matrix         | HNO <sub>3</sub> / HF |                |              |
| <b>Analyte</b> | <b>µg/mL</b>          | <b>Analyte</b> | <b>µg/mL</b> |
| B              | 100                   | Sb             | 100          |
| Ge             | 100                   | Si             | 100          |
| Hf             | 100                   | Sn             | 100          |
| Mo             | 100                   | Ta             | 100          |
| Nb             | 100                   | Ti             | 100          |
| P              | 100                   | W              | 100          |
| Re             | 100                   | Zr             | 100          |
| S              | 100                   |                |              |

**Transition ICP-MS Standard**

|                |                  |                |              |
|----------------|------------------|----------------|--------------|
| CCS-6          |                  |                |              |
| Volume         | 125 mL           |                |              |
| Matrix         | HNO <sub>3</sub> |                |              |
| <b>Analyte</b> | <b>µg/mL</b>     | <b>Analyte</b> | <b>µg/mL</b> |
| Ag             | 100              | Mn             | 100          |
| Cd             | 100              | Ni             | 100          |
| Co             | 100              | Pb             | 100          |
| Cr             | 100              | Tl             | 100          |
| Cu             | 100              | V              | 100          |
| Fe             | 100              | Zn             | 100          |
| Hg             | 100              |                |              |

**Tellurium ICP-MS Standard**

|                |                  |
|----------------|------------------|
| MSTEN-100PPM   |                  |
| Volume         | 125 mL           |
| Matrix         | HNO <sub>3</sub> |
| <b>Analyte</b> | <b>µg/mL</b>     |
| Te             | 100              |

## Calibration Standards (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

### 71-Element Group

#### ICP-MS Complete Standard

##### IV-ICPMS-71A

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Lu      | 10    |
| Al      | 10    | Mg      | 10    |
| As      | 10    | Mn      | 10    |
| B       | 10    | Na      | 10    |
| Ba      | 10    | Nd      | 10    |
| Be      | 10    | Ni      | 10    |
| Ca      | 10    | P       | 10    |
| Cd      | 10    | Pb      | 10    |
| Ce      | 10    | Pr      | 10    |
| Co      | 10    | Rb      | 10    |
| Cr      | 10    | S       | 10    |
| Cs      | 10    | Se      | 10    |
| Cu      | 10    | Sm      | 10    |
| Dy      | 10    | Sr      | 10    |
| Er      | 10    | Th      | 10    |
| Eu      | 10    | Tl      | 10    |
| Fe      | 10    | Tm      | 10    |
| Ga      | 10    | U       | 10    |
| Gd      | 10    | V       | 10    |
| Ho      | 10    | Yb      | 10    |
| K       | 10    | Zn      | 10    |
| La      | 10    |         |       |

#### Lithium ICP-MS Standard

##### MSLI-10PPM

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL |
|---------|-------|
| Li      | 10    |

#### ICP-MS Refractory Elements Standard

##### IV-ICPMS-71B

Volume 125 mL  
Matrix HNO<sub>3</sub> / HF

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ge      | 10    | Sn      | 10    |
| Hf      | 10    | Ta      | 10    |
| Mo      | 10    | Te      | 10    |
| Nb      | 10    | Ti      | 10    |
| Sb      | 10    | W       | 10    |
| Si      | 10    | Zr      | 10    |

#### ICP-MS Precious Metals Standard

##### IV-ICPMS-71C

Volume 125 mL  
Matrix HCl

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Au      | 10    | Pt      | 10    |
| Ir      | 10    | Re      | 10    |
| Os      | 10    | Rh      | 10    |
| Pd      | 10    | Ru      | 10    |

#### ICP-MS Mercury

##### MSHG-10PPM

Volume 125 mL  
Matrix HCl

| Analyte | µg/mL |
|---------|-------|
| Hg      | 10    |

#### ICP-MS Internal Standard

##### IV-ICPMS-71D

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 10    | Sc      | 10    |
| In              | 10    | Tb      | 10    |
| <sup>6</sup> Li | 10    | Y       | 10    |

### Well-versed...

I have never had problems with Inorganic Ventures' standards, both mixed and multi-element. Your prompt delivery of standards is well within the time that I need the material. The labeling of standards is also quite good. I also find your website most informative, from calculations to general information.

*Jules Bitay  
Morristown, NJ*



## Calibration Standards (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

### VAR Calibration Standard 1

#### VAR-CAL-1

Volume 125 mL  
Matrix HNO<sub>3</sub> / HF

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Mo      | 100   | Sn      | 100   |
| Sb      | 100   | Ti      | 100   |

### VAR Calibration Standard 2

#### VAR-CAL-2

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Mn      | 100   |
| Al      | 100   | Ni      | 100   |
| As      | 100   | Pb      | 100   |
| Ba      | 100   | Se      | 100   |
| Be      | 100   | Th      | 100   |
| Cd      | 100   | Tl      | 100   |
| Co      | 100   | U       | 100   |
| Cr      | 100   | V       | 100   |
| Cu      | 100   | Zn      | 100   |

### PE Calibration Standard 3

#### PE-CAL-3

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ca      | 1000  | Tl      | 1000  |
| Fe      | 1000  | Y       | 1000  |
| Li      | 1000  |         |       |

### GENESIS Calibration Standard 4

#### GENESIS-ICAL

Volume 125 mL  
Matrix HNO<sub>3</sub> / HCl

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Be      | 2     | Na      | 5     |
| Ca      | 1     | Ni      | 10    |
| Ce      | 10    | P       | 10    |
| Cu      | 10    | S       | 50    |
| Eu      | 10    | Sc      | 5     |
| Fe      | 10    | Si      | 10    |
| In      | 10    | Sr      | 2     |
| K       | 10    | Ti      | 10    |
| Li      | 2     | V       | 10    |
| Mn      | 5     | Y       | 10    |
| Mo      | 5     | Zr      | 10    |

### VAR Calibration Standard 7

#### VAR-CAL-7

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Al               | 5     | Mn      | 5     |
| As               | 5     | Mo      | 5     |
| Ba               | 5     | Ni      | 5     |
| Cd               | 5     | Pb      | 5     |
| Co               | 5     | Se      | 5     |
| Cr <sup>+3</sup> | 5     | Sr      | 5     |
| Cu               | 5     | Zn      | 5     |
| K                | 50    |         |       |

*"Our focus is to give the highest level of technical support and customer service, making your loyalty our greatest success."*

**Christopher Gaines**  
Vice President of Operations



**Calibration Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**ICP Calibration Standard 1**

## IV-STOCK-1

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 50    | Fe      | 15    |
| Al               | 100   | Ga      | 150   |
| B                | 15    | In      | 200   |
| Ba               | 5     | Mn      | 5     |
| Be               | 1     | Ni      | 50    |
| Bi               | 200   | Pb      | 200   |
| Cd               | 20    | Sr      | 1     |
| Co               | 20    | Tl      | 400   |
| Cr <sup>+3</sup> | 25    | Zn      | 20    |
| Cu               | 20    |         |       |

**ICP Calibration Standard 2**

## IV-STOCK-2

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL  | Analyte | µg/mL  |
|---------|--------|---------|--------|
| Ca      | 10,000 | Mg      | 10,000 |
| K       | 10,000 | Na      | 10,000 |

**ICP Calibration Standard 3**

## IV-STOCK-3

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ca      | 1,000 | Mg      | 1,000 |
| K       | 1,000 | Na      | 1,000 |

**ICP Calibration Standard 4**

## IV-STOCK-4

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 1,000 | In      | 1,000 |
| Al               | 1,000 | K       | 1,000 |
| B                | 1,000 | Li      | 1,000 |
| Ba               | 1,000 | Mg      | 1,000 |
| Bi               | 1,000 | Mn      | 1,000 |
| Ca               | 1,000 | Na      | 1,000 |
| Cd               | 1,000 | Ni      | 1,000 |
| Co               | 1,000 | Pb      | 1,000 |
| Cr <sup>+3</sup> | 1,000 | Sr      | 1,000 |
| Cu               | 1,000 | Tl      | 1,000 |
| Fe               | 1,000 | Zn      | 1,000 |
| Ga               | 1,000 |         |       |

**ICP Calibration Standard 8**

## IV-STOCK-8

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Al               | 100   | K       | 100   |
| B                | 100   | Li      | 100   |
| Ba               | 100   | Mg      | 100   |
| Be               | 100   | Mn      | 100   |
| Bi               | 100   | Na      | 100   |
| Ca               | 100   | Ni      | 100   |
| Cd               | 100   | Pb      | 100   |
| Co               | 100   | Se      | 100   |
| Cr <sup>+3</sup> | 100   | Sr      | 100   |
| Cu               | 100   | Te      | 100   |
| Fe               | 100   | Tl      | 100   |
| Ga               | 100   | Zn      | 100   |

**Supportive...**

Inorganic Ventures gives us fast, reliable service with stock and custom standards. Your customer representatives are ALWAYS courteous and friendly. Additionally, your standards and QC are always high quality. And it is never a problem to speak with your top technicians. Thank you for your prompt, courteous, friendly, and reliable service.

Jeff Graham  
Hattiesburg, MS

## Calibration Standards (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

### ICP Calibration Standard - Toxic Elements

#### IV-STOCK-9

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Pb      | 100   |
| Be      | 100   | Se      | 100   |
| Cd      | 100   | Tl      | 100   |
| Ni      | 100   |         |       |

### ICP Calibration Standard - Surface Water

#### IV-STOCK-10

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/L   | Analyte | µg/L   |
|------------------|--------|---------|--------|
| As               | 50     | Mg      | 15,000 |
| B                | 100    | Mn      | 30     |
| Ba               | 50     | Mo      | 100    |
| Be               | 20     | Na      | 8,000  |
| Bi               | 10     | Ni      | 50     |
| Ca               | 35,000 | Pb      | 25     |
| Cd               | 20     | Se      | 10     |
| Co               | 25     | Sr      | 100    |
| Cr <sup>3+</sup> | 20     | Tl      | 10     |
| Cu               | 20     | V       | 50     |
| Fe               | 100    | Zn      | 50     |
| K                | 3,000  |         |        |

### ICP Calibration Standard - Sewage Sludge

#### IV-STOCK-11

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Cd               | 10    | Ni      | 200   |
| Cr <sup>3+</sup> | 900   | Pb      | 900   |
| Cu               | 800   | Zn      | 2,500 |

### ICP Calibration Standard - Trace Metals

#### IV-STOCK-13

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Al               | 500   | Fe      | 100   |
| As               | 100   | Mn      | 100   |
| Be               | 100   | Ni      | 100   |
| Cd               | 25    | Pb      | 100   |
| Co               | 100   | Se      | 25    |
| Cr <sup>3+</sup> | 100   | V       | 250   |
| Cu               | 100   | Zn      | 100   |

### ICP Calibration Standard - Earth Alkali Element

#### IV-STOCK-16

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ba      | 1000  | Mg      | 1000  |
| Ca      | 1000  | Sr      | 1000  |

### ICP-MS Calibration Standard 6

#### IV-STOCK-6

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 10    | Li      | 10    |
| Al               | 10    | Mg      | 10    |
| As               | 100   | Mn      | 10    |
| B                | 100   | Mo      | 10    |
| Ba               | 10    | Na      | 10    |
| Be               | 100   | Ni      | 10    |
| Bi               | 10    | Pb      | 10    |
| Ca               | 1000  | Rb      | 10    |
| Cd               | 10    | Se      | 100   |
| Co               | 10    | Sr      | 10    |
| Cr <sup>3+</sup> | 10    | Te      | 10    |
| Cu               | 10    | Tl      | 10    |
| Fe               | 100   | U       | 10    |
| Ga               | 10    | V       | 10    |
| K                | 10    | Zn      | 100   |

**Calibration Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**ICP-MS Calibration Standard 15**

## IV-STOCK-15

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ca      | 10    | Li      | 10    |
| Fe      | 10    | Na      | 10    |
| K       | 10    |         |       |

**ICP-MS Calibration Standard 22**

## IV-STOCK-22

Volume 125 mL  
Matrix HNO<sub>3</sub> / HCl

**NEW**

| Analyte | µg/L | Analyte | µg/L |
|---------|------|---------|------|
| Cd      | 200  | Pb      | 200  |
| Cu      | 200  | Rh      | 200  |
| Mg      | 200  |         |      |

**ICP Calibration Standard - HCl Soluble Elements**

## IV-STOCK-17

Volume 125 mL  
Matrix HNO<sub>3</sub> / HCl / HF

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Hf      | 100   | Ta      | 100   |
| Ir      | 100   | Ti      | 100   |
| Sb      | 100   | Zr      | 100   |
| Sn      | 100   |         |       |

**ICP-MS Calibration Standard 23**

## IV-STOCK-23

Volume 500 mL  
Matrix HNO<sub>3</sub> / HCl

**NEW**

| Analyte | µg/L | Analyte | µg/L |
|---------|------|---------|------|
| B       | 1    | Lu      | 1    |
| Ba      | 1    | Na      | 1    |
| Co      | 1    | Rh      | 1    |
| Fe      | 1    | Sc      | 1    |
| Ga      | 1    | Tl      | 1    |
| In      | 1    | U       | 1    |
| K       | 1    | Y       | 1    |
| Li      | 1    |         |      |

**ICP-MS Calibration Standard 21**

## IV-STOCK-21

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 10    | K       | 10    |
| Al               | 10    | Li      | 10    |
| As               | 10    | Mg      | 10    |
| Ba               | 10    | Mn      | 10    |
| Be               | 10    | Na      | 10    |
| Bi               | 10    | Ni      | 10    |
| Ca               | 10    | Pb      | 10    |
| Cd               | 10    | Rb      | 10    |
| Co               | 10    | Se      | 10    |
| Cr <sup>+3</sup> | 10    | Sr      | 10    |
| Cs               | 10    | Tl      | 10    |
| Cu               | 10    | U       | 10    |
| Fe               | 10    | V       | 10    |
| Ga               | 10    | Zn      | 10    |
| In               | 10    |         |       |

**ICP-MS Calibration Standard 26**

## IV-STOCK-26

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ce      | 10    | Pr      | 10    |
| Dy      | 10    | Sc      | 10    |
| Er      | 10    | Sm      | 10    |
| Eu      | 10    | Tb      | 10    |
| Gd      | 10    | Th      | 10    |
| Ho      | 10    | Tm      | 10    |
| La      | 10    | Y       | 10    |
| Lu      | 10    | Yb      | 10    |
| Nd      | 10    |         |       |

**Calibration Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**ICP-MS Calibration Standard 27**

## IV-STOCK-27

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 10    | Li      | 10    |
| Al               | 10    | Mg      | 10    |
| As               | 10    | Mn      | 10    |
| Ba               | 10    | Na      | 10    |
| Be               | 10    | Ni      | 10    |
| Ca               | 10    | Pb      | 10    |
| Cd               | 10    | Rb      | 10    |
| Co               | 10    | Se      | 10    |
| Cr <sup>+3</sup> | 10    | Sr      | 10    |
| Cs               | 10    | Tl      | 10    |
| Cu               | 10    | U       | 10    |
| Fe               | 10    | V       | 10    |
| Ga               | 10    | Zn      | 10    |
| K                | 10    |         |       |

**ICP-MS Calibration Standard 28**

## IV-STOCK-28

Volume 125 mL  
Matrix HCl / HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Au      | 10    | Rh      | 10    |
| Hf      | 10    | Ru      | 10    |
| Ir      | 10    | Sb      | 10    |
| Pd      | 10    | Sn      | 10    |
| Pt      | 10    | Te      | 10    |

**ICP-MS Calibration Standard 29**

## IV-STOCK-29

Volume 125 mL  
Matrix HNO<sub>3</sub> / HF

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| B       | 10    | S       | 10    |
| Ge      | 10    | Si      | 10    |
| Mo      | 10    | Ta      | 10    |
| Nb      | 10    | Ti      | 10    |
| P       | 10    | W       | 10    |
| Re      | 10    | Zr      | 10    |

**ICP-MS Calibration Standard 30**

## IV-STOCK-30

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Be      | 10    | Mg      | 10    |
| Bi      | 10    | Ni      | 10    |
| Ce      | 10    | Pb      | 10    |
| Co      | 10    | U       | 10    |
| In      | 10    |         |       |


**ICP-MS Calibration Standard 31**

## IV-STOCK-31

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Al      | 1     | Mg      | 0.2   |
| Ba      | 0.2   | Mn      | 1     |
| Ca      | 0.2   | Ni      | 5     |
| Cu      | 1     | P       | 10    |
| K       | 5     | Zn      | 0.2   |

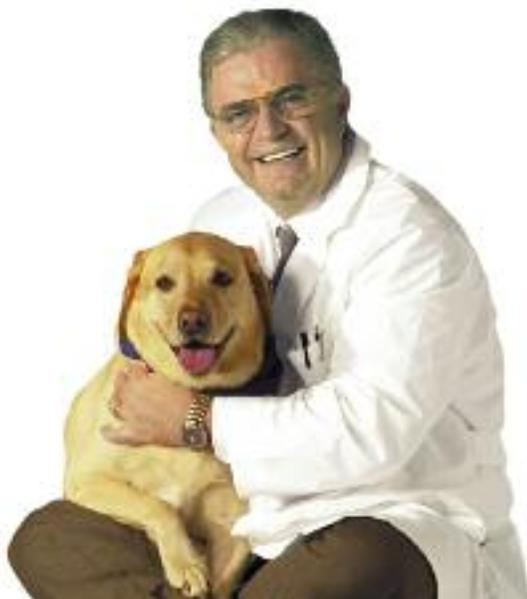

*"We're here to help every lab, big and small."*

**Paul R. Gaines, Ph.D.**  
CEO & Fellow Chemist

**Calibration Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**ICP-MS Calibration Standard 33**

## IV-STOCK-33

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ca      | 500   | Mg      | 500   |
| Fe      | 500   | Na      | 500   |
| K       | 500   |         |       |

**VAR Internal Standard Solution**

## VAR-IS-1

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 100   | Sc      | 100   |
| In              | 100   | Tb      | 100   |
| <sup>6</sup> Li | 100   | Y       | 100   |

**ICP-MS Detection Limit Standard**

## IV-STOCK-19

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/L | Analyte | µg/L |
|---------|------|---------|------|
| Be      | 10   | Tl      | 10   |
| Co      | 10   | U       | 10   |
| In      | 10   |         |      |

**Trace Metals in Water**

## IV-STOCK-1643

Volume 125 mL  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/L   | Analyte | µg/L   |
|------------------|--------|---------|--------|
| Ag               | 1      | Mg      | 8,000  |
| Al               | 142    | Mn      | 39     |
| As               | 60     | Mo      | 121    |
| B                | 158    | Na      | 21,000 |
| Ba               | 544    | Ni      | 62     |
| Be               | 14     | Pb      | 20     |
| Bi               | 14     | Rb      | 14     |
| Ca               | 32,000 | Re      | 113    |
| Cd               | 7      | Sb      | 58     |
| Co               | 27     | Se      | 12     |
| Cr <sup>3+</sup> | 20     | Sr      | 323    |
| Cu               | 23     | Te      | 1      |
| Fe               | 98     | Tl      | 7      |
| K                | 2,000  | V       | 38     |
| Li               | 17     | Zn      | 79     |

**ICP-MS Plasma Setup Solution**

## IV-STOCK-20

Volume 1 Liter  
Matrix HNO<sub>3</sub>

**NEW**

| Analyte | µg/L | Analyte | µg/L |
|---------|------|---------|------|
| Ba      | 10   | Pb      | 10   |
| Cd      | 10   | Rh      | 10   |
| Ce      | 10   | Sc      | 10   |
| Cu      | 10   | Tb      | 10   |
| Ge      | 10   | Tl      | 10   |
| Mg      | 10   |         |      |

**PE Check Standard 1**

## PE-CHK-1

Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Mn      | 10    |
| Al      | 10    | Ni      | 10    |
| As      | 10    | Pb      | 10    |
| Ba      | 10    | Sb      | 10    |
| Be      | 10    | Se      | 10    |
| Cd      | 10    | Tl      | 10    |
| Co      | 10    | V       | 10    |
| Cr      | 10    | Zn      | 10    |
| Cu      | 10    |         |       |

## Wavelength Calibration Standards (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

### Wavelength Calibration Standard 1

#### IV-STOCK-5

Volume 500 mL  
Matrix HCl

**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Al               | 20    | Mg      | 1     |
| As               | 20    | Mn      | 1     |
| B                | 2     | Na      | 20    |
| Ba               | 2     | Ni      | 5     |
| Be               | 1     | P       | 10    |
| Ca               | 10    | Pb      | 20    |
| Cd               | 2     | Sc      | 1     |
| Cr <sup>+3</sup> | 2     | Se      | 20    |
| Cu               | 2     | Sr      | 1     |
| Fe               | 2     | Te      | 20    |
| Hg               | 5     | Ti      | 2     |
| K                | 100   | Y       | 1     |
| Li               | 2     | Zn      | 2     |

### Wavelength Calibration Standard 2

#### IV-STOCK-14

Volume 500 mL  
Matrix HCl tr HNO<sub>3</sub>

**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 20    | Na      | 20    |
| K       | 100   | Ni      | 20    |
| La      | 20    | P       | 100   |
| Li      | 20    | S       | 100   |
| Mn      | 20    | Sc      | 20    |
| Mo      | 20    |         |       |

## Tuning Solution Standards

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

### PE Tuning Solution

#### PE-TS-1

Volume 125 mL  
Matrix HNO<sub>3</sub> / HCl

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ba      | 10    | Mg      | 10    |
| Be      | 10    | Pb      | 10    |
| Ce      | 10    | Rh      | 10    |
| Co      | 10    | Tl      | 10    |
| In      | 10    | U       | 10    |
| Li      | 10    | Y       | 10    |

### AGI Tuning Solution

#### AGI-TS-1

Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ce      | 10    | Tl      | 10    |
| Co      | 10    | Y       | 10    |
| Li      | 10    |         |       |

### CIROS Tuning Solution

#### CIROS-OES-TS

Volume 125 mL  
Matrix HCl / HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Fe      | 10    | P       | 10    |
| K       | 10    | S       | 50    |
| La      | 10    | Sc      | 10    |
| Mg      | 5     | Ti      | 10    |
| Mn      | 5     |         |       |

### THM Tuning Solution

#### THM-TS-1

Volume 125 mL  
Matrix HNO<sub>3</sub> tr HCl

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| B       | 10    | K       | 10    |
| Ba      | 10    | Rh      | 10    |
| Co      | 10    | Sc      | 10    |
| Ga      | 10    | Na      | 10    |
| In      | 10    | Th      | 10    |
| Fe      | 10    | U       | 10    |
| Li      | 10    | Y       | 10    |
| Lu      | 10    |         |       |

**Tuning Solution Standards** (continued)

Don't see what you need? Contact us with the solution part number and instrument manufacturer you're seeking and we'll give you a very competitive price!

**VAR Tuning Solution**

## VAR-TS-MS

Volume 125 mL

Matrix HNO<sub>3</sub>

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ba      | 10    | Mg      | 10    |
| Be      | 10    | Pb      | 10    |
| Ce      | 10    | Th      | 10    |
| Co      | 10    | Tl      | 10    |
| In      | 10    |         |       |

**Stock Tuning Solution 12**

## IV-STOCK-12

Volume 125 mL

Matrix HNO<sub>3</sub>**NEW**

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ba      | 10    | In      | 10    |
| Be      | 10    | Li      | 10    |
| Bi      | 10    | Ni      | 10    |
| Ce      | 10    | Pb      | 10    |
| Co      | 10    | U       | 10    |

**Stock Tuning Solution 24**

## IV-STOCK-24

Volume 500 mL

Matrix HNO<sub>3</sub>**NEW**

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Al               | 50    | Mn      | 50    |
| As               | 50    | Mo      | 50    |
| Ba               | 50    | Ni      | 50    |
| Cd               | 50    | Pb      | 50    |
| Co               | 50    | Se      | 50    |
| Cr <sup>+3</sup> | 50    | Sr      | 50    |
| Cu               | 50    | Zn      | 50    |
| K                | 500   |         |       |

**Cost-effective...**

We needed a 9-element standard with varying concentrations. Inorganic Ventures' ability to do this meant we did not have to prepare it ourselves. It was inexpensive and reliable.

Michael Clark  
Springfield, MO

*"Our pride shows in every standard we make."*

**Vin DeAngelo**  
Packaging Technician



## HIGH-PURITY IONIZATION BUFFERS

Ionization buffers are 99.999+% pure. They are analyzed using both axial-view ICP-OES and ICP-MS for 70+ impurities. Custom ionization buffers are available upon request.

## 1% Cesium Ionization Buffer

CSN-ISB-5  
Volume 500 mL  
Matrix HNO<sub>3</sub>

Analyte  $\mu\text{g/mL}$

Cs 10,000

High Purity buffer; ideal for Axial View ICP-OES

## 2% Lithium Ionization Buffer

LINB2-5  
Volume 500 mL  
Matrix HNO<sub>3</sub>

Analyte  $\mu\text{g/mL}$

Li 20,000

## 5% Cesium Ionization Buffer

CSN-ISB5-5  
Volume 500 mL  
Matrix HNO<sub>3</sub>

Analyte  $\mu\text{g/mL}$

Cs 50,000

## 1% Potassium Ionization Buffer

KN-ISB-5  
Volume 500 mL  
Matrix Water/HCl

Analyte  $\mu\text{g/mL}$

K 10,000

## EPA STANDARDS

## ILMO3.0

Standards for ILMO3.0 are designed for use with ICP-OES. Custom EPA standards are available upon request.

## Calibration Standards

## Calibration Standard 1

CLPP-CAL-1  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | $\mu\text{g/mL}$ | Analyte | $\mu\text{g/mL}$ |
|---------|------------------|---------|------------------|
| Ag      | 250              | Fe      | 1000             |
| Al      | 2000             | K       | 5000             |
| Ba      | 2000             | Mg      | 5000             |
| Be      | 50               | Mn      | 500              |
| Ca      | 5000             | Na      | 5000             |
| Co      | 500              | Ni      | 500              |
| Cr      | 200              | V       | 500              |
| Cu      | 250              | Zn      | 500              |

## Calibration Standard 2

CGSB1-1  
Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100

| Analyte | $\mu\text{g/mL}$ |
|---------|------------------|
| Sb      | 1000             |

## Calibration Standard 3

CLPP-CAL-3  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | $\mu\text{g/mL}$ | Analyte | $\mu\text{g/mL}$ |
|---------|------------------|---------|------------------|
| As      | 1000             | Se      | 1000             |
| Cd      | 500              | Tl      | 1000             |
| Pb      | 1000             |         |                  |

## ILMO3.0 (continued)

### CICV Standards

CICV - Continuing and Initial Calibration Verification.

#### CICV Standard 1<sup>†</sup>

##### QCP-CICV-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 125   | Fe      | 500   |
| Al      | 1000  | K       | 2500  |
| Ba      | 1000  | Mg      | 2500  |
| Be      | 25    | Mn      | 250   |
| Ca      | 2500  | Na      | 2500  |
| Co      | 250   | Ni      | 250   |
| Cr      | 100   | V       | 250   |
| Cu      | 125   | Zn      | 250   |

#### CICV Standard 2<sup>†</sup>

##### QCP-CICV-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100 or 1:500

| Analyte | µg/mL |
|---------|-------|
| Sb      | 500   |

#### CICV Standard 3<sup>†</sup>

##### QCP-CICV-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 500   | Se      | 500   |
| Cd      | 250   | Tl      | 500   |
| Pb      | 500   |         |       |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

### CRDL Standards

CRDL - Contract Required Detection Limit.

#### CRDL Standard 1

##### CRI-CRA-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 200   | Mn      | 300   |
| Be      | 100   | Ni      | 800   |
| Co      | 1000  | V       | 1000  |
| Cr      | 200   | Zn      | 400   |
| Cu      | 500   |         |       |

#### CRDL Standard 2

##### CRI-CRA-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Sb      | 600   |

#### CRDL Standard 3

##### CRI-CRA-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Se      | 50    |
| Cd      | 50    | Tl      | 100   |
| Pb      | 30    |         |       |

### Interference Check Standards

#### Interference Check Standard A

##### CLPP-ICS-A

Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Al      | 5000  | Fe      | 2000  |
| Ca      | 5000  | Mg      | 5000  |

#### Interference Check Standard B

##### CLPP-ICS-B

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Cu      | 50    |
| Ba      | 50    | Mn      | 50    |
| Be      | 50    | Ni      | 100   |
| Cd      | 100   | Pb      | 100   |
| Co      | 50    | V       | 50    |
| Cr      | 50    | Zn      | 100   |

**ILMO3.0** (continued)**Soil & Water Spike Standards****Spike Standard 1\***

CLPP-SPK-1

Volume 125 mL

Matrix HNO<sub>3</sub>

Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 50    | Cu      | 250   |
| Al      | 2000  | Fe      | 1000  |
| Ba      | 2000  | Mn      | 500   |
| Be      | 50    | Ni      | 500   |
| Co      | 500   | V       | 500   |
| Cr      | 200   | Zn      | 500   |

**Spike Standard 2\***

CLPP-SPK-2

Volume 125 mL

Matrix HNO<sub>3</sub> / Tartaric Acid

Dilution 1:1000

| Analyte | µg/mL |
|---------|-------|
| Sb      | 500   |

**Spike Standard 3\***

CLPP-SPK-3

Volume 125 mL

Matrix HNO<sub>3</sub>

Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 2000  | Se      | 2000  |
| Cd      | 50    | Tl      | 2000  |
| Pb      | 500   |         |       |

\*Instructions included.

**ILMO4.0**

Standards for ILMO4.0 are designed for use with ICP-OES. Custom EPA standards are available upon request.

**Calibration Standards****Calibration Standard 1**

CLPP-CAL-1

Volume 125 mL

Matrix HNO<sub>3</sub>

Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 250   | Fe      | 1000  |
| Al      | 2000  | K       | 5000  |
| Ba      | 2000  | Mg      | 5000  |
| Be      | 50    | Mn      | 500   |
| Ca      | 5000  | Na      | 5000  |
| Co      | 500   | Ni      | 500   |
| Cr      | 200   | V       | 500   |
| Cu      | 250   | Zn      | 500   |

**Calibration Standard 2**

CGSB1-1

Volume 125 mL

Matrix HNO<sub>3</sub> / Tartaric Acid

Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Sb      | 1000  |

**Calibration Standard 3**

CLPP-CAL-3

Volume 125 mL

Matrix HNO<sub>3</sub>

Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 1000  | Se      | 1000  |
| Cd      | 500   | Tl      | 1000  |
| Pb      | 1000  |         |       |

## ILMO4.0 (continued)

### CICV Standards

CICV - Continuing and Initial Calibration Verification.

#### CICV Standard 1<sup>†</sup>

##### QCP-CICV-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 125   | Fe      | 500   |
| Al      | 1000  | K       | 2500  |
| Ba      | 1000  | Mg      | 2500  |
| Be      | 25    | Mn      | 250   |
| Ca      | 2500  | Na      | 2500  |
| Co      | 250   | Ni      | 250   |
| Cr      | 100   | V       | 250   |
| Cu      | 125   | Zn      | 250   |

#### CICV Standard 2<sup>†</sup>

##### QCP-CICV-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100 or 1:500

| Analyte | µg/mL |
|---------|-------|
| Sb      | 500   |

#### CICV Standard 3<sup>†</sup>

##### QCP-CICV-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 500   | Se      | 500   |
| Cd      | 250   | Tl      | 500   |
| Pb      | 500   |         |       |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

### CRDL Standards

CRDL - Contract Required Detection Limit.

#### CRDL Standard 1

##### CRI-CRA-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 200   | Mn      | 300   |
| Be      | 100   | Ni      | 800   |
| Co      | 1000  | V       | 1000  |
| Cr      | 200   | Zn      | 400   |
| Cu      | 500   |         |       |

#### CRDL Standard 2

##### CRI-CRA-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Sb      | 600   |

#### CRDL Standard 3

##### CRI-CRA-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Se      | 50    |
| Cd      | 50    | Tl      | 100   |
| Pb      | 30    |         |       |

### Interference Check Standards

#### Interference Check Standard A

##### CLPP-ICS-A

Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Al      | 5000  | Fe      | 2000  |
| Ca      | 5000  | Mg      | 5000  |

#### Interference Check Standard B4

##### CLPP-ICS-B4

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mn      | 50    |
| As      | 10    | Ni      | 100   |
| Ba      | 50    | Pb      | 5     |
| Be      | 50    | Sb      | 60    |
| Cd      | 100   | Se      | 5     |
| Co      | 50    | Tl      | 10    |
| Cr      | 50    | V       | 50    |
| Cu      | 50    | Zn      | 100   |

**ILMO4.0** (continued)**Soil & Water Spike Standards****Spike Standard 1\***

## CLPP-SPK-1

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:1000           |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 50    | Cu      | 250   |
| Al      | 2000  | Fe      | 1000  |
| Ba      | 2000  | Mn      | 500   |
| Be      | 50    | Ni      | 500   |
| Co      | 500   | V       | 500   |
| Cr      | 200   | Zn      | 500   |

**Spike Standard 4\***

## CLPP-SPK-4

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:1000           |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 40    | Sb      | 100   |
| Cd      | 50    | Se      | 10    |
| Pb      | 20    | Tl      | 50    |

\*Instructions included.

**ILMO5.2 & ILMO5.3**

See individual products for recommended instrumentation and revision. Custom EPA standards are available upon request.

**Calibration Standards****Calibration Standard 1**

## CLPP-CAL-1

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 250   | Fe      | 1000  |
| Al      | 2000  | K       | 5000  |
| Ba      | 2000  | Mg      | 5000  |
| Be      | 50    | Mn      | 500   |
| Ca      | 5000  | Na      | 5000  |
| Co      | 500   | Ni      | 500   |
| Cr      | 200   | V       | 500   |
| Cu      | 250   | Zn      | 500   |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

**Calibration Standard 2**

## CGSB1-1

|          |                                  |
|----------|----------------------------------|
| Volume   | 125 mL                           |
| Matrix   | HNO <sub>3</sub> / Tartaric Acid |
| Dilution | 1:100                            |

| Analyte | µg/mL |
|---------|-------|
| Sb      | 1000  |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

**Calibration Standard 3**

## CLPP-CAL-3

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 1000  | Se      | 1000  |
| Cd      | 500   | Tl      | 1000  |
| Pb      | 1000  |         |       |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

**Calibration Standard 4**

## CLP-MS-CAL

|          |                                  |
|----------|----------------------------------|
| Volume   | 125 mL                           |
| Matrix   | HNO <sub>3</sub> / Tartaric Acid |
| Dilution | 1:100 to 1:1000                  |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mg      | 20    |
| Al      | 20    | Mn      | 20    |
| As      | 20    | Ni      | 20    |
| Ba      | 20    | Pb      | 20    |
| Be      | 20    | Sb      | 20    |
| Cd      | 20    | Se      | 20    |
| Co      | 20    | Tl      | 20    |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 20    |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

## ILMO5.2 & ILMO5.3 (continued)

### CICV Standards

CICV - Continuing and Initial Calibration Verification.

#### CICV Standard 1<sup>†</sup>

##### QCP-CICV-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 125   | Fe      | 500   |
| Al      | 1000  | K       | 2500  |
| Ba      | 1000  | Mg      | 2500  |
| Be      | 25    | Mn      | 250   |
| Ca      | 2500  | Na      | 2500  |
| Co      | 250   | Ni      | 250   |
| Cr      | 100   | V       | 250   |
| Cu      | 125   | Zn      | 250   |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

#### CICV Standard 2<sup>†</sup>

##### QCP-CICV-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100 or 1:500

| Analyte | µg/mL |
|---------|-------|
| Sb      | 500   |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

#### CICV Standard 3<sup>†</sup>

##### QCP-CICV-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 or 1:500

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 500   | Se      | 500   |
| Cd      | 250   | Tl      | 500   |
| Pb      | 500   |         |       |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

<sup>†</sup>Manufactured from in-house Second Source concentrates.

#### CICV Standard 4<sup>†</sup>

##### CLP-MS-CICV

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Mg      | 10    |
| Al      | 10    | Mn      | 10    |
| As      | 10    | Ni      | 10    |
| Ba      | 10    | Pb      | 10    |
| Be      | 10    | Sb      | 10    |
| Cd      | 10    | Se      | 10    |
| Co      | 10    | Tl      | 10    |
| Cr      | 10    | V       | 10    |
| Cu      | 10    | Zn      | 10    |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### CICV Standard 5<sup>†</sup>

##### QCP-ICV-1REV

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Mn      | 10    |
| Al      | 10    | Ni      | 10    |
| As      | 10    | Pb      | 10    |
| Ba      | 10    | Sb      | 10    |
| Be      | 10    | Se      | 10    |
| Cd      | 10    | Tl      | 10    |
| Co      | 10    | V       | 10    |
| Cr      | 10    | Zn      | 10    |
| Cu      | 10    |         |       |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

*"All of us are constantly striving to flex to your specs in everything we do."*

**Jhiam Marasigan**  
Accounting Supervisor



## ILMO5.2 &amp; ILMO5.3 (continued)

## CRDL &amp; CRQL Standards

CRDL - Contract Required Detection Limit. CRQL - Contract Required Quantitation Limit.

## CRDL Standard

CLP-AES-CRDL  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
|---------|-------|---------|-------|

See [inorganicventures.com](http://inorganicventures.com) for analytes.

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

## CRQL Standard 1

CLP-AES-CRQL  
 Volume 125 mL  
 Matrix HNO<sub>3</sub> / Tartaric Acid  
 Dilution 1:100 (water samples); 1:500 (soil samples)

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 1     | K       | 500   |
| Al      | 20    | Mg      | 500   |
| As      | 1.5   | Mn      | 1.5   |
| Ba      | 20    | Na      | 500   |
| Be      | 0.5   | Ni      | 4     |
| Ca      | 500   | Pb      | 1     |
| Cd      | 0.5   | Sb      | 6     |
| Co      | 5     | Se      | 3.5   |
| Cr      | 1     | Tl      | 2.5   |
| Cu      | 2.5   | V       | 5     |
| Fe      | 10    | Zn      | 6     |

For use with ICP-OES. Designed for ILMO5.2.

## CRQL Standard 2

CLP-AES-CRQL-2  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:100 (water samples); 1:500 (soil samples)

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 1     | K       | 500   |
| Al      | 20    | Mg      | 500   |
| As      | 1     | Mn      | 1.5   |
| Ba      | 20    | Na      | 500   |
| Be      | 0.5   | Ni      | 4     |
| Ca      | 500   | Pb      | 1     |
| Cd      | 0.5   | Sb      | 6     |
| Co      | 5     | Se      | 3.5   |
| Cr      | 1     | Tl      | 2.5   |
| Cu      | 2.5   | V       | 5     |
| Fe      | 10    | Zn      | 6     |

For use with ICP-OES. Designed for ILMO5.3.

## CRQL Standard 3

CLP-MS-CRQL  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 1     | Mn      | 0.5   |
| Al      | 30    | Ni      | 1     |
| As      | 1     | Pb      | 1     |
| Ba      | 10    | Sb      | 2     |
| Be      | 1     | Se      | 5     |
| Cd      | 1     | Tl      | 1     |
| Co      | 5     | V       | 1     |
| Cr      | 2     | Zn      | 1     |
| Cu      | 1     |         |       |

For use with ICP-MS. Designed for ILMO5.2.

## CRQL Standard 4

CLP-MS-CRQL-2  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 1     | Mn      | 1     |
| As      | 1     | Ni      | 1     |
| Ba      | 10    | Pb      | 1     |
| Be      | 1     | Sb      | 2     |
| Cd      | 1     | Se      | 5     |
| Co      | 1     | Tl      | 1     |
| Cr      | 2     | V       | 1     |
| Cu      | 2     | Zn      | 2     |

For use with ICP-MS. Designed for ILMO5.3.

## CRQL Standard 5

CLP-MS-CRQL-3  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 1     | Mn      | 1     |
| As      | 1     | Ni      | 1     |
| Ba      | 10    | Pb      | 1     |
| Be      | 1     | Sb      | 2     |
| Cd      | 1     | Se      | 5     |
| Co      | 1     | Tl      | 1     |
| Cr      | 2     | V       | 5     |
| Cu      | 2     | Zn      | 2     |

## ILMO5.2 & ILMO5.3 (continued)

### Interference Check Standards

#### Interference Check Standard A

CLPP-ICS-A  
Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Al      | 5000  | Fe      | 2000  |
| Ca      | 5000  | Mg      | 5000  |

For use with ICP-OES and ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### Interference Check Standard B

CLPP-ICS-B  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 2     | Mg      | 2     |
| Al      | 2     | Mn      | 2     |
| As      | 2     | Ni      | 2     |
| Ba      | 2     | Pb      | 2     |
| Be      | 2     | Sb      | 2     |
| Cd      | 2     | Se      | 2     |
| Co      | 2     | Tl      | 2     |
| Cr      | 2     | V       | 2     |
| Cu      | 2     | Zn      | 2     |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### Interference Check Standard B4

CLPP-ICS-B4  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mn      | 50    |
| As      | 10    | Ni      | 100   |
| Ba      | 50    | Pb      | 5     |
| Be      | 50    | Sb      | 60    |
| Cd      | 100   | Se      | 5     |
| Co      | 50    | Tl      | 10    |
| Cr      | 50    | V       | 50    |
| Cu      | 50    | Zn      | 100   |

For use with ICP-OES. Designed for ILMO5.2 and ILMO5.3.

### Soil & Water Spike Standards

#### Spike Standard

CLP-MS-SPK  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 5     | Mn      | 50    |
| Al      | 200   | Ni      | 50    |
| As      | 4     | Pb      | 2     |
| Ba      | 200   | Sb      | 10    |
| Be      | 5     | Se      | 1     |
| Cd      | 5     | Tl      | 5     |
| Co      | 50    | V       | 50    |
| Cr      | 20    | Zn      | 50    |
| Cu      | 25    |         |       |

For use with ICP-MS. Instructions included. Designed for ILMO5.2 and ILMO5.3.

#### Spike Standard 1

CLPP-SPK-1  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 50    | Cu      | 250   |
| Al      | 2000  | Fe      | 1000  |
| Ba      | 2000  | Mn      | 500   |
| Be      | 50    | Ni      | 500   |
| Co      | 500   | V       | 500   |
| Cr      | 200   | Zn      | 500   |


For use with ICP-OES. Instructions included. Designed for ILMO5.2 and ILMO5.3.

#### Spike Standard 5

CLPP-SPK-5  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 40    | Sb      | 100   |
| Cd      | 50    | Se      | 50    |
| Pb      | 20    | Tl      | 50    |

For use with ICP-OES. Instructions included. Designed for ILMO5.2 and ILMO5.3.

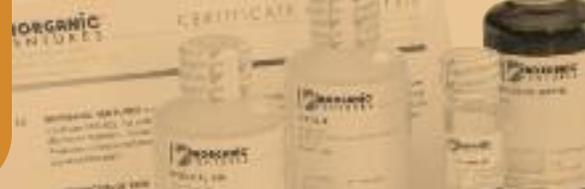

## ILMO5.2 & ILMO5.3 (continued)

### Internal Standards & Tuning Solutions

#### Internal Standard

6020ISS  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 10    | Rh      | 10    |
| Ho              | 10    | Sc      | 10    |
| In              | 10    | Tb      | 10    |
| <sup>6</sup> Li | 10    | Y       | 10    |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### Tuning Solution

6020TS  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Co      | 10    | Li      | 10    |
| In      | 10    | Tl      | 10    |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### Tuning Solution

2008TS  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Be      | 10    | Mg      | 10    |
| Co      | 10    | Pb      | 10    |
| In      | 10    |         |       |

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

### Blank & Rinse Solutions

Blank & rinse solutions are prepared using double-distilled nitric acid and ASTM Type 1 water. They come packaged in ultra-clean LDPE bottles.

#### 1% (v/v) Nitric Acid Calibration Blank

CLP-MS-BLANK  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution RTU

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

#### 2% (v/v) Nitric Acid Rinse

CLP-MS-RINSE  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution RTU

For use with ICP-MS. Designed for ILMO5.2 and ILMO5.3.

### Customer-focused...

Inorganic Ventures has always provided us with fast, reliable and friendly service during a time when great customer service is becoming the exception rather than the rule. Thanks Inorganic Ventures!

*Julie Dickerson*  
Largo, MD

## Method 200.7

Standards for Method 200.7 are designed for use with ICP-OES.  
Custom EPA standards are available upon request.

### 200.7 Calibration

Standards designed for Method 200.7 (1982), Method 3120, Method 6010A Rev. 1, and Method 200.7 CLP-M.

#### Calibration Standard 1A

WW-CAL-1A  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Ag      | 50    | 328.068 |
| As      | 1000  | 193.759 |
| B       | 100   | 249.678 |
| Ba      | 100   | 493.409 |
| Ca      | 1000  | 315.887 |
| Cd      | 200   | 226.502 |
| Cu      | 200   | 324.754 |
| Mn      | 200   | 257.610 |
| Se      | 500   | 196.090 |
| Sr      | 100   | 421.552 |

NOTE: Sr does not exhibit spectral interference problems with any of the EPA Method 200.7 analytes.

#### Calibration Standard 1B

CLPP-SPK-2  
Volume 125 mL  
Matrix HNO<sub>3</sub> / Tartaric Acid  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Sb      | 500   | 206.833 |

#### Calibration Standard 2

WW-CAL-2  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| K       | 2000  | 766.491 |
| Li      | 500   | 670.784 |
| Mo      | 1000  | 203.844 |
| Na      | 1000  | 588.995 |
| Ti      | 1000  | 334.941 |

#### Calibration Standard 3

WW-CAL-3  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Ce      | 200   | 413.765 |
| Co      | 200   | 228.616 |
| P       | 1000  | 214.914 |
| V       | 200   | 292.402 |

#### Calibration Standard 4A

WW-CAL-4A  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Al      | 1000  | 308.215 |
| Cr      | 500   | 205.552 |
| Hg      | 200   | 194.227 |
| Zn      | 500   | 213.856 |

#### Calibration Standard 4B

WW-CAL-4B  
Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte          | µg/mL | λ(nm)   |
|------------------|-------|---------|
| SiO <sub>2</sub> | 1000  | 251.611 |
| Sn               | 400   | 189.980 |

#### Calibration Standard 5

WW-CAL-5  
Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Be      | 100   | 313.042 |
| Fe      | 1000  | 259.940 |
| Mg      | 1000  | 279.079 |
| Ni      | 200   | 231.604 |
| Pb      | 1000  | 220.353 |
| Tl      | 500   | 190.864 |

## Method 200.7 (continued)

## 200.7 Interference Checks

## Interference Check Standard 1

2007ICS-1  
 Volume 125 mL  
 Matrix HNO<sub>3</sub> / HF  
 Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| B       | 500   | Si      | 230   |
| Mo      | 300   | Ti      | 1000  |

## Interference Check Standard 2

CGSB1-1  
 Volume 125 mL  
 Matrix HNO<sub>3</sub> / Tartaric Acid  
 Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Sb      | 1000  |

## Interference Check Standard 3

2007ICS-3  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL  |
|---------|-------|---------|--------|
| Ag      | 300   | K       | 20,000 |
| As      | 1000  | Mn      | 200    |
| Ba      | 300   | Ni      | 300    |
| Be      | 100   | Pb      | 1000   |
| Cd      | 300   | Se      | 500    |
| Co      | 300   | Tl      | 1000   |
| Cr      | 300   | V       | 300    |
| Cu      | 300   | Zn      | 300    |

## Interference Check Standard 4

2007ICS-4  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:50

| Analyte | µg/mL  | Analyte | µg/mL |
|---------|--------|---------|-------|
| Al      | 3000   | Mg      | 7500  |
| Ca      | 15,000 | Na      | 2500  |
| Fe      | 12,500 |         |       |

## 200.7 Quality Controls

Quality Control Standard 1<sup>†</sup>

QCP-QCS-1  
 Volume 125 mL  
 Matrix HNO<sub>3</sub>  
 Dilution 1:100

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Ag      | 25    | 328.068 |
| Al      | 100   | 308.215 |
| As      | 200   | 193.759 |
| B       | 100   | 249.678 |
| Ba      | 100   | 493.409 |
| Be      | 100   | 313.042 |
| Ca      | 100   | 315.887 |
| Cd      | 100   | 226.502 |
| Ce      | 100   | 413.765 |
| Co      | 100   | 228.616 |
| Cr      | 100   | 205.552 |
| Cu      | 100   | 324.754 |
| Fe      | 100   | 259.940 |
| Hg      | 200   | 194.227 |
| K       | 500   | 766.491 |
| Li      | 100   | 670.784 |
| Mg      | 100   | 279.079 |
| Mn      | 100   | 257.610 |
| Na      | 100   | 588.995 |
| Ni      | 100   | 231.604 |
| P       | 500   | 214.914 |
| Pb      | 200   | 220.353 |
| Se      | 100   | 196.099 |
| Sr      | 100   | 421.552 |
| Tl      | 500   | 190.864 |
| V       | 100   | 292.402 |
| Zn      | 100   | 213.856 |

Quality Control Standard 2<sup>†</sup>

QCP-QCS-2  
 Volume 125 mL  
 Matrix HNO<sub>3</sub> / HF  
 Dilution 1:100

| Analyte          | µg/mL | λ (nm)  |
|------------------|-------|---------|
| Mo               | 100   | 203.844 |
| Sb               | 200   | 206.833 |
| SiO <sub>2</sub> | 500   | 251.611 |
| Sn               | 500   | 189.980 |
| Ti               | 100   | 334.941 |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

## Method 200.7 (continued)

### 200.7 Quality Controls (continued)

#### Quality Control Standard 7<sup>†</sup>

IV-7  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | K       | 1000  |
| Al      | 100   | Na      | 100   |
| B       | 100   | Si      | 50    |
| Ba      | 100   |         |       |

#### Quality Control Standard 19<sup>†</sup>

IV-19  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Mo      | 100   |
| Be      | 100   | Ni      | 100   |
| Ca      | 100   | Pb      | 100   |
| Cd      | 100   | Sb      | 100   |
| Co      | 100   | Se      | 100   |
| Cr      | 100   | Ti      | 100   |
| Cu      | 100   | Tl      | 100   |
| Fe      | 100   | V       | 100   |
| Mg      | 100   | Zn      | 100   |
| Mn      | 100   |         |       |

#### Quality Control Standard 21<sup>†</sup>

IV-21  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Mo      | 100   |
| Be      | 100   | Ni      | 100   |
| Ca      | 100   | Pb      | 100   |
| Cd      | 100   | Sb      | 100   |
| Co      | 100   | Se      | 100   |
| Cr      | 100   | Sr      | 100   |
| Cu      | 100   | Ti      | 100   |
| Fe      | 100   | Tl      | 100   |
| Li      | 100   | V       | 100   |
| Mg      | 100   | Zn      | 100   |
| Mn      | 100   |         |       |

#### Quality Control Standard 26<sup>†</sup>

IV-26  
Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Mg      | 100   |
| Al      | 100   | Mn      | 100   |
| As      | 100   | Mo      | 100   |
| B       | 100   | Na      | 100   |
| Ba      | 100   | Ni      | 100   |
| Be      | 100   | Pb      | 100   |
| Ca      | 100   | Sb      | 100   |
| Cd      | 100   | Se      | 100   |
| Co      | 100   | Si      | 50    |
| Cr      | 100   | Ti      | 100   |
| Cu      | 100   | Tl      | 100   |
| Fe      | 100   | V       | 100   |
| K       | 1000  | Zn      | 100   |

#### Quality Control Standard 28<sup>†</sup>

IV-28  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Mg      | 100   |
| Al      | 100   | Mn      | 100   |
| As      | 100   | Mo      | 100   |
| B       | 100   | Na      | 100   |
| Ba      | 100   | Ni      | 100   |
| Be      | 100   | Pb      | 100   |
| Ca      | 100   | Sb      | 100   |
| Cd      | 100   | Se      | 100   |
| Co      | 100   | Si      | 50    |
| Cr      | 100   | Sr      | 100   |
| Cu      | 100   | Ti      | 100   |
| Fe      | 100   | Tl      | 100   |
| K       | 1000  | V       | 100   |
| Li      | 100   | Zn      | 100   |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

**Method 200.7** (continued)**Rev. 3.3 & 4.4 Calibrations**

Standards may be used for either revision.

**Calibration Standard 1A**

## WW-CAL-1A

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Ag      | 50    | 328.068 |
| As      | 1000  | 193.759 |
| B       | 100   | 249.678 |
| Ba      | 100   | 493.409 |
| Ca      | 1000  | 315.887 |
| Cd      | 200   | 226.502 |
| Cu      | 200   | 324.754 |
| Mn      | 200   | 257.610 |
| Se      | 500   | 196.090 |
| Sr      | 100   | 421.552 |

NOTE: Sr does not exhibit spectral interference problems with any of the EPA Method 200.7 analytes.

**Calibration Standard 1B**

## CLPP-SPK-2

|          |                                  |
|----------|----------------------------------|
| Volume   | 125 mL                           |
| Matrix   | HNO <sub>3</sub> / Tartaric Acid |
| Dilution | 1:100                            |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Sb      | 500   | 206.833 |

**Calibration Standard 2**

## WW-CAL-2

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| K       | 2000  | 766.491 |
| Li      | 500   | 670.784 |
| Mo      | 1000  | 203.844 |
| Na      | 1000  | 588.995 |
| Ti      | 1000  | 334.941 |

**Calibration Standard 3**

## WW-CAL-3

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Ce      | 200   | 413.765 |
| Co      | 200   | 228.616 |
| P       | 1000  | 214.914 |
| V       | 200   | 292.402 |

**Calibration Standard 4A**

## WW-CAL-4A

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Al      | 1000  | 308.215 |
| Cr      | 500   | 205.552 |
| Hg      | 200   | 194.227 |
| Zn      | 500   | 213.856 |

**Calibration Standard 4B**

## WW-CAL-4B

|          |                       |
|----------|-----------------------|
| Volume   | 125 mL                |
| Matrix   | HNO <sub>3</sub> / HF |
| Dilution | 1:100                 |

| Analyte          | µg/mL | λ (nm)  |
|------------------|-------|---------|
| SiO <sub>2</sub> | 1000  | 251.611 |
| Sn               | 400   | 189.980 |

**Calibration Standard 5**

## WW-CAL-5

|          |                       |
|----------|-----------------------|
| Volume   | 125 mL                |
| Matrix   | HNO <sub>3</sub> / HF |
| Dilution | 1:100                 |

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Be      | 100   | 313.042 |
| Fe      | 1000  | 259.940 |
| Mg      | 1000  | 279.079 |
| Ni      | 200   | 231.604 |
| Pb      | 1000  | 220.353 |
| Tl      | 500   | 190.864 |

## Method 200.7 (continued)

### Rev. 3.3 & 4.4 Instrument Performance Checks

#### Instrument Performance Check 1

##### WW-IPC-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Ag      | 25    | 328.068 |
| Al      | 200   | 308.215 |
| As      | 200   | 193.759 |
| B       | 200   | 249.678 |
| Ba      | 200   | 493.409 |
| Be      | 200   | 313.042 |
| Ca      | 200   | 315.887 |
| Cd      | 200   | 226.502 |
| Ce      | 200   | 413.765 |
| Co      | 200   | 228.616 |
| Cr      | 200   | 205.552 |
| Cu      | 200   | 324.754 |
| Fe      | 200   | 259.940 |
| Hg      | 200   | 194.227 |
| K       | 1000  | 766.491 |
| Li      | 200   | 670.784 |
| Mg      | 200   | 279.079 |
| Mn      | 200   | 257.610 |
| Na      | 200   | 588.995 |
| Ni      | 200   | 231.604 |
| P       | 1000  | 214.914 |
| Pb      | 200   | 220.353 |
| Se      | 200   | 196.090 |
| Sr      | 200   | 421.552 |
| Tl      | 200   | 190.864 |
| V       | 200   | 292.402 |
| Zn      | 200   | 213.856 |

#### Instrument Performance Check 3

##### WW-IPC-3

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | λ (nm)  |
|---------|-------|---------|
| Ag      | 25    | 328.068 |
| Al      | 200   | 308.215 |
| As      | 200   | 193.759 |
| B       | 200   | 249.678 |
| Ba      | 200   | 493.409 |
| Be      | 200   | 313.042 |
| Ca      | 200   | 315.887 |
| Cd      | 200   | 226.502 |
| Co      | 200   | 228.616 |
| Cr      | 200   | 205.552 |
| Cu      | 200   | 324.754 |
| Fe      | 200   | 259.940 |
| K       | 1000  | 766.491 |
| Li      | 200   | 670.784 |
| Mg      | 200   | 279.079 |
| Mn      | 200   | 257.610 |
| Na      | 200   | 588.995 |
| Ni      | 200   | 231.604 |
| P       | 1000  | 214.914 |
| Pb      | 200   | 220.353 |
| Se      | 200   | 196.090 |
| Sr      | 200   | 421.552 |
| Tl      | 200   | 190.864 |
| V       | 200   | 292.402 |
| Zn      | 200   | 213.856 |

#### Instrument Performance Check 2

##### WW-IPC-2

Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte          | µg/mL | λ (nm)  |
|------------------|-------|---------|
| Mo               | 200   | 203.844 |
| Sb               | 200   | 206.833 |
| SiO <sub>2</sub> | 1000  | 251.611 |
| Sn               | 200   | 189.980 |
| Ti               | 200   | 334.941 |

*"The sky's the limit when it comes to satisfying our customers!"*

**Denise Bottazzi**  
Manufacturing Technician



## Method 200.7 (continued)

## Rev. 3.3 &amp; 4.4 Laboratory Fortified Stocks

## Laboratory Fortified Stock Solution 1

## WW-LFS-1

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Ag      | 7.5   | 328.068 |
| Al      | 200   | 308.215 |
| As      | 80    | 193.759 |
| B       | 30    | 249.678 |
| Ba      | 20    | 493.409 |
| Be      | 20    | 313.042 |
| Ca      | 100   | 315.887 |
| Cd      | 20    | 226.502 |
| Ce      | 200   | 413.765 |
| Co      | 20    | 228.616 |
| Cr      | 40    | 205.552 |
| Cu      | 30    | 324.754 |
| Fe      | 300   | 259.940 |
| Hg      | 70    | 194.227 |
| K       | 1000  | 766.491 |
| Li      | 20    | 670.784 |
| Mg      | 200   | 279.079 |
| Mn      | 20    | 257.610 |
| Na      | 300   | 588.995 |
| Ni      | 50    | 231.604 |
| P       | 600   | 214.914 |
| Pb      | 100   | 220.353 |
| Se      | 200   | 196.090 |
| Sr      | 20    | 421.552 |
| Tl      | 200   | 190.864 |
| V       | 30    | 292.402 |
| Zn      | 20    | 213.856 |

## Laboratory Fortified Stock Solution 2

## WW-LFS-2

|          |                       |
|----------|-----------------------|
| Volume   | 125 mL                |
| Matrix   | HNO <sub>3</sub> / HF |
| Dilution | 1:100                 |

| Analyte          | µg/mL | λ(nm)   |
|------------------|-------|---------|
| Mo               | 40    | 203.844 |
| Sb               | 80    | 206.833 |
| SiO <sub>2</sub> | 200   | 251.611 |
| Sn               | 70    | 189.980 |
| Ti               | 20    | 334.941 |

## Rev. 3.3 &amp; 4.4 Quality Controls

Quality Control Standard 1<sup>†</sup>

## QCP-QCS-1

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | λ(nm)   |
|---------|-------|---------|
| Ag      | 25    | 328.068 |
| Al      | 100   | 308.215 |
| As      | 200   | 193.759 |
| B       | 100   | 249.678 |
| Ba      | 100   | 493.409 |
| Be      | 100   | 313.042 |
| Ca      | 100   | 315.887 |
| Cd      | 100   | 226.502 |
| Ce      | 100   | 413.765 |
| Co      | 100   | 228.616 |
| Cr      | 100   | 205.552 |
| Cu      | 100   | 324.754 |
| Fe      | 100   | 259.940 |
| Hg      | 200   | 194.227 |
| K       | 500   | 766.491 |
| Li      | 100   | 670.784 |
| Mg      | 100   | 279.079 |
| Mn      | 100   | 257.610 |
| Na      | 100   | 588.995 |
| Ni      | 100   | 231.604 |
| P       | 500   | 214.914 |
| Pb      | 200   | 220.353 |
| Se      | 100   | 196.099 |
| Sr      | 100   | 421.552 |
| Tl      | 500   | 190.864 |
| V       | 100   | 292.402 |
| Zn      | 100   | 213.856 |

Quality Control Standard 2<sup>†</sup>

## QCP-QCS-2

|          |                       |
|----------|-----------------------|
| Volume   | 125 mL                |
| Matrix   | HNO <sub>3</sub> / HF |
| Dilution | 1:100                 |

| Analyte          | µg/mL | λ(nm)   |
|------------------|-------|---------|
| Mo               | 100   | 203.844 |
| Sb               | 200   | 206.833 |
| SiO <sub>2</sub> | 500   | 251.611 |
| Sn               | 500   | 189.980 |
| Ti               | 100   | 334.941 |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

## Method 200.7 (continued)

### Rev. 3.3 & 4.4 Quality Controls (continued)

#### Quality Control Standard 7<sup>†</sup>

IV-7  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | K       | 1000  |
| Al      | 100   | Na      | 100   |
| B       | 100   | Si      | 50    |
| Ba      | 100   |         |       |

#### Quality Control Standard 19<sup>†</sup>

IV-19  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Mo      | 100   |
| Be      | 100   | Ni      | 100   |
| Ca      | 100   | Pb      | 100   |
| Cd      | 100   | Sb      | 100   |
| Co      | 100   | Se      | 100   |
| Cr      | 100   | Ti      | 100   |
| Cu      | 100   | Tl      | 100   |
| Fe      | 100   | V       | 100   |
| Mg      | 100   | Zn      | 100   |
| Mn      | 100   |         |       |

#### Quality Control Standard 21<sup>†</sup>

IV-21  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 100   | Mo      | 100   |
| Be      | 100   | Ni      | 100   |
| Ca      | 100   | Pb      | 100   |
| Cd      | 100   | Sb      | 100   |
| Co      | 100   | Se      | 100   |
| Cr      | 100   | Sr      | 100   |
| Cu      | 100   | Ti      | 100   |
| Fe      | 100   | Tl      | 100   |
| Li      | 100   | V       | 100   |
| Mg      | 100   | Zn      | 100   |
| Mn      | 100   |         |       |

#### Quality Control Standard 26<sup>†</sup>

IV-26  
Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Mg      | 100   |
| Al      | 100   | Mn      | 100   |
| As      | 100   | Mo      | 100   |
| B       | 100   | Na      | 100   |
| Ba      | 100   | Ni      | 100   |
| Be      | 100   | Pb      | 100   |
| Ca      | 100   | Sb      | 100   |
| Cd      | 100   | Se      | 100   |
| Co      | 100   | Si      | 50    |
| Cr      | 100   | Ti      | 100   |
| Cu      | 100   | Tl      | 100   |
| Fe      | 100   | V       | 100   |
| K       | 1000  | Zn      | 100   |

#### Quality Control Standard 28<sup>†</sup>

IV-28  
Volume 125 mL  
Matrix HNO<sub>3</sub> tr HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 100   | Mg      | 100   |
| Al      | 100   | Mn      | 100   |
| As      | 100   | Mo      | 100   |
| B       | 100   | Na      | 100   |
| Ba      | 100   | Ni      | 100   |
| Be      | 100   | Pb      | 100   |
| Ca      | 100   | Sb      | 100   |
| Cd      | 100   | Se      | 100   |
| Co      | 100   | Si      | 50    |
| Cr      | 100   | Sr      | 100   |
| Cu      | 100   | Ti      | 100   |
| Fe      | 100   | Tl      | 100   |
| K       | 1000  | V       | 100   |
| Li      | 100   | Zn      | 100   |

<sup>†</sup>Manufactured from in-house Second Source concentrates.



## Method 200.8

Standards for Method 200.8 are designed for use with ICP-MS.  
Custom EPA standards are available upon request.

### Rev. 4.4 & 5.4 Calibration

See individual products for recommended revisions.

#### Calibration Standard 1

2008CAL-1  
Volume 125 mL  
Matrix HNO<sub>3</sub> / HF  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Mo      | 20    | Sb      | 20    |

Designed for Rev. 4.4 and Rev. 5.4.

#### Calibration Standard 2

2008CAL-2  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mn      | 20    |
| Al      | 20    | Ni      | 20    |
| As      | 20    | Pb      | 20    |
| Ba      | 20    | Se      | 20    |
| Be      | 20    | Th      | 20    |
| Cd      | 20    | Tl      | 20    |
| Co      | 20    | U       | 20    |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 20    |

Designed for Rev. 4.4.

#### Calibration Standard 2A

WW-MSCAL-2  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mn      | 20    |
| Al      | 20    | Ni      | 20    |
| As      | 20    | Pb      | 20    |
| Ba      | 20    | Se      | 100   |
| Be      | 20    | Th      | 20    |
| Cd      | 20    | Tl      | 20    |
| Co      | 20    | U       | 20    |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 20    |

Designed for Rev. 5.4.

#### Calibration Standard 3

WW-MSCAL-1  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:1000

| Analyte | µg/mL |
|---------|-------|
| Hg      | 5     |

Designed for Rev. 5.4.



*"Our goal at Inorganic Ventures is to provide the best customer service world wide. We always guarantee 100% satisfaction!"*

**Noelle Newman**  
International Sales

## Method 200.8 (continued)

### Rev. 4.4 & 5.4 Internal Standards

#### Internal Standard

2008ISS  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Bi      | 20    | Tb      | 20    |
| In      | 20    | Y       | 20    |
| Sc      | 20    |         |       |

Designed for Rev. 4.4 and 5.4. Recommended working level is 200 µg/L for Rev. 4.4; 20-200 µg/L for Rev. 5.4. Use this solution with CGAUN1-1 for Rev. 5.4 if Hg is to be determined by direct analysis.

#### Mercury Preservation Solution

CGAUN1-1  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Au      | 1000  |

Designed for Rev. 5.4. Add an aliquot of this solution to 2008ISS, sufficient to provide a concentration of 100 µg/L in the final dilution of all blanks, calibration standards, and samples.

### Rev. 4.4 & 5.4 Quality Controls

#### Quality Control Standard 3<sup>†</sup>

QCP-QCS-3  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Mn      | 10    |
| Al      | 10    | Mo      | 10    |
| As      | 10    | Na      | 10    |
| Ba      | 10    | Ni      | 10    |
| Be      | 10    | Pb      | 10    |
| Ca      | 10    | Sb      | 10    |
| Cd      | 10    | Se      | 50    |
| Co      | 10    | Th      | 10    |
| Cr      | 10    | Tl      | 10    |
| Cu      | 10    | U       | 10    |
| Fe      | 10    | V       | 10    |
| K       | 10    | Zn      | 10    |
| Mg      | 10    |         |       |

Designed for Rev. 4.4 and Rev. 5.4.

#### Quality Control Standard 4<sup>†</sup>

QCP-QCS-4  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL |
|---------|-------|
| Hg      | 5     |

Designed for Rev. 4.4 and Rev. 5.4.

<sup>†</sup>Manufactured from in-house Second Source concentrates

### Rev. 4.4 & 5.4 Tuning

#### Tuning Solution

2008TS  
Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Be      | 10    | Mg      | 10    |
| Co      | 10    | Pb      | 10    |
| In      | 10    |         |       |

Designed for Rev. 4.4 and Rev. 5.4.

### Fast...

One thing that Inorganic Ventures never fails at is a timely delivery. When I, or any of my associates, place an order—whether it be via telephone or internet—it is received normally within 1-2 business days. I wish more companies had quick turnaround like that!

Susan Hogan  
La Verne, CA

## Method 6020

Standards for Method 6020 are designed for use with ICP-MS.  
Custom EPA standards are available upon request.

### CLP-M Version 8

#### Calibration Standard

##### 6020CAL-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | K       | 20    |
| Al      | 20    | Mg      | 20    |
| As      | 20    | Mn      | 20    |
| Ba      | 20    | Na      | 20    |
| Be      | 20    | Ni      | 20    |
| Ca      | 20    | Pb      | 20    |
| Cd      | 20    | Sb      | 20    |
| Co      | 20    | Se      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 20    | Zn      | 20    |

#### Interference Check Standard A

##### 6020ICS-8A

Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte         | µg/mL  | Analyte | µg/mL |
|-----------------|--------|---------|-------|
| Al              | 1000   | Mg      | 1000  |
| C               | 2000   | Mo      | 20    |
| Ca              | 3000   | Na      | 2500  |
| Cl <sup>-</sup> | 18,000 | P       | 1000  |
| Fe              | 2500   | S       | 1000  |
| K               | 1000   | Ti      | 20    |

#### Interference Check Standard B

##### 6020ICS-8B

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mn      | 20    |
| As      | 10    | Ni      | 20    |
| Cd      | 10    | Se      | 10    |
| Co      | 20    | V       | 20    |
| Cr      | 20    | Zn      | 10    |
| Cu      | 20    |         |       |

#### Internal Standard

##### 6020ISS

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 10    | Rh      | 10    |
| Ho              | 10    | Sc      | 10    |
| In              | 10    | Tb      | 10    |
| <sup>6</sup> Li | 10    | Y       | 10    |

#### Memory Check Standard 1

##### 6020MCC-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:2

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mg      | 1000  |
| Al      | 1000  | Mn      | 20    |
| As      | 20    | Mo      | 20    |
| Ba      | 20    | Na      | 1000  |
| Be      | 20    | Ni      | 20    |
| C       | 2000  | Pb      | 20    |
| Ca      | 1000  | Sb      | 20    |
| Cd      | 20    | Se      | 20    |
| Co      | 20    | Ti      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 1000  | Zn      | 20    |
| K       | 1000  |         |       |

NOTE: For use with 6020MCC-2. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for his method.

#### Memory Check Standard 2

##### 6020MCC-2

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:2

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Cl <sup>-</sup> | 7200  | S       | 1000  |
| P               | 1000  |         |       |

NOTE: For use with 6020MCC-1. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for this method.

## Method 6020 (continued)

### CLP-M Version 8 (continued)

#### Spike Standard - Soil

##### 6020SPK-S

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Ni      | 25    |
| As      | 10    | Pb      | 20    |
| Ba      | 50    | Sb      | 20    |
| Be      | 5     | Se      | 5     |
| Cd      | 10    | Tl      | 5     |
| Co      | 20    | V       | 30    |
| Cr      | 50    | Zn      | 50    |
| Cu      | 50    |         |       |

#### Spike Standard - Water

##### 6020SPK-W

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 5     | Mn      | 20    |
| As      | 10    | Ni      | 20    |
| Ba      | 50    | Pb      | 10    |
| Be      | 5     | Sb      | 20    |
| Cd      | 5     | Se      | 5     |
| Co      | 20    | Tl      | 5     |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 50    |
| Fe      | 100   |         |       |

#### Tuning Solution

##### 6020TS

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Co      | 10    | Li      | 10    |
| In      | 10    | Tl      | 10    |

### CLP-M Version 9

#### Calibration Standard

##### 6020CAL-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | K       | 20    |
| Al      | 20    | Mg      | 20    |
| As      | 20    | Mn      | 20    |
| Ba      | 20    | Na      | 20    |
| Be      | 20    | Ni      | 20    |
| Ca      | 20    | Pb      | 20    |
| Cd      | 20    | Sb      | 20    |
| Co      | 20    | Se      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 20    | Zn      | 20    |

#### Interference Check Standard A

##### 6020ICS-9A

Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte         | µg/mL  | Analyte | µg/mL |
|-----------------|--------|---------|-------|
| Al              | 1000   | Mg      | 1000  |
| C               | 2000   | Mo      | 20    |
| Ca              | 3000   | Na      | 2500  |
| Cl <sup>-</sup> | 21,215 | P       | 1000  |
| Fe              | 2500   | S       | 1000  |
| K               | 1000   | Ti      | 20    |

#### Interference Check Standard B

##### 6020ICS-9B

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 5     | Mn      | 20    |
| As      | 10    | Ni      | 20    |
| Cd      | 10    | Se      | 10    |
| Co      | 20    | V       | 20    |
| Cr      | 20    | Zn      | 10    |
| Cu      | 20    |         |       |

**Method 6020** (continued)**CLP-M Version 9** (continued)**Internal Standard****6020ISS**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 10    | Rh      | 10    |
| Ho              | 10    | Sc      | 10    |
| In              | 10    | Tb      | 10    |
| <sup>6</sup> Li | 10    | Y       | 10    |

**Memory Check Standard 1****6020MCC-1**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:2              |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mg      | 1000  |
| Al      | 1000  | Mn      | 20    |
| As      | 20    | Mo      | 20    |
| Ba      | 20    | Na      | 1000  |
| Be      | 20    | Ni      | 20    |
| C       | 2000  | Pb      | 20    |
| Ca      | 1000  | Sb      | 20    |
| Cd      | 20    | Se      | 20    |
| Co      | 20    | Ti      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 1000  | Zn      | 20    |
| K       | 1000  |         |       |

NOTE: For use with 6020MCC-2. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for this method.

**Memory Check Standard 2****6020MCC-2**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:2              |

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Cl <sup>-</sup> | 7200  | S       | 1000  |
| P               | 1000  |         |       |

NOTE: For use with 6020MCC-1. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for this method.

**Spike Standard - Soil****6020SPK-S**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Ni      | 25    |
| As      | 10    | Pb      | 20    |
| Ba      | 50    | Sb      | 20    |
| Be      | 5     | Se      | 5     |
| Cd      | 10    | Tl      | 5     |
| Co      | 20    | V       | 30    |
| Cr      | 50    | Zn      | 50    |
| Cu      | 50    |         |       |

**Spike Standard - Water****6020SPK-W**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 5     | Mn      | 20    |
| As      | 10    | Ni      | 20    |
| Ba      | 50    | Pb      | 10    |
| Be      | 5     | Sb      | 20    |
| Cd      | 5     | Se      | 5     |
| Co      | 20    | Tl      | 5     |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 50    |
| Fe      | 100   |         |       |

**Tuning Solution****6020TS**

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Co      | 10    | Li      | 10    |
| In      | 10    | Tl      | 10    |

## Method 6020 (continued)

### Rev. 0

#### Calibration Standard

##### 6020CAL-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | K       | 20    |
| Al      | 20    | Mg      | 20    |
| As      | 20    | Mn      | 20    |
| Ba      | 20    | Na      | 20    |
| Be      | 20    | Ni      | 20    |
| Ca      | 20    | Pb      | 20    |
| Cd      | 20    | Sb      | 20    |
| Co      | 20    | Se      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 20    | Zn      | 20    |

#### CICV Standard 5<sup>†</sup>

##### QCP-ICV-1REV

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100 to 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Mn      | 10    |
| Al      | 10    | Ni      | 10    |
| As      | 10    | Pb      | 10    |
| Ba      | 10    | Sb      | 10    |
| Be      | 10    | Se      | 10    |
| Cd      | 10    | Tl      | 10    |
| Co      | 10    | V       | 10    |
| Cr      | 10    | Zn      | 10    |
| Cu      | 10    |         |       |

<sup>†</sup> Manufactured from in-house Second Source concentrates.

#### Interference Check Standard A

##### 6020ICS-0A

Volume 500 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte         | µg/mL  | Analyte | µg/mL |
|-----------------|--------|---------|-------|
| Al              | 1000   | Mg      | 1000  |
| C               | 2000   | Mo      | 20    |
| Ca              | 1000   | Na      | 1000  |
| Cl <sup>-</sup> | 10,000 | P       | 1000  |
| Fe              | 1000   | S       | 1000  |
| K               | 1000   | Ti      | 20    |

#### Interference Check Standard B

##### 6020ICS-0B

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 2     | Cu      | 2     |
| As      | 2     | Mn      | 2     |
| Cd      | 2     | Ni      | 2     |
| Co      | 2     | Zn      | 2     |
| Cr      | 2     |         |       |

#### Internal Standard

##### 6020ISS

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Bi              | 10    | Rh      | 10    |
| Ho              | 10    | Sc      | 10    |
| In              | 10    | Tb      | 10    |
| <sup>6</sup> Li | 10    | Y       | 10    |

## Accurate...

We'll question any analysis that we determine to be outside of the norm. But we never question the ICP standards we receive from Inorganic Ventures. Thanks for supplying a quality product at a fair price.

*Kevin Campbell  
Rock Hill, SC*



## Method 6020 (continued)

Rev. 0 (continued)

### Memory Check Standard 1

#### 6020MCC-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:2

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 20    | Mg      | 1000  |
| Al      | 1000  | Mn      | 20    |
| As      | 20    | Mo      | 20    |
| Ba      | 20    | Na      | 1000  |
| Be      | 20    | Ni      | 20    |
| C       | 2000  | Pb      | 20    |
| Ca      | 1000  | Sb      | 20    |
| Cd      | 20    | Se      | 20    |
| Co      | 20    | Ti      | 20    |
| Cr      | 20    | Tl      | 20    |
| Cu      | 20    | V       | 20    |
| Fe      | 1000  | Zn      | 20    |
| K       | 1000  |         |       |

NOTE: For use with 6020MCC-2. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for this method.

### Memory Check Standard 2

#### 6020MCC-2

Volume 125 mL  
Matrix H<sub>2</sub>O  
Dilution 1:2

| Analyte         | µg/mL | Analyte | µg/mL |
|-----------------|-------|---------|-------|
| Cl <sup>-</sup> | 7200  | S       | 1000  |
| P               | 1000  |         |       |

NOTE: For use with 6020MCC-1. When combined, these concentrates will precipitate. The precipitate will not adversely effect the results for this method.



*"We're always searching for new ways to improve our services and website with all eyes on flexing to your specs."*

**Brian Brolin**  
Director of Marketing and E-commerce

### Spike Standard - Soil

#### 6020SPK-S

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 10    | Ni      | 25    |
| As      | 10    | Pb      | 20    |
| Ba      | 50    | Sb      | 20    |
| Be      | 5     | Se      | 5     |
| Cd      | 10    | Tl      | 5     |
| Co      | 20    | V       | 30    |
| Cr      | 50    | Zn      | 50    |
| Cu      | 50    |         |       |

### Spike Standard - Water

#### 6020SPK-W

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 5     | Mn      | 20    |
| As      | 10    | Ni      | 20    |
| Ba      | 50    | Pb      | 10    |
| Be      | 5     | Sb      | 20    |
| Cd      | 5     | Se      | 5     |
| Co      | 20    | Tl      | 5     |
| Cr      | 20    | V       | 20    |
| Cu      | 20    | Zn      | 50    |
| Fe      | 100   |         |       |

### Tuning Solution

#### 6020TS

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Co      | 10    | Li      | 10    |
| In      | 10    | Tl      | 10    |

# ION CHROMATOGRAPHY



If you've been searching for an atypical Ion Chromatography standard, look no further. Over the years, we've developed the most complete line of IC standards on the market. Our technicians have stabilized more than a dozen rare anion and cation standards that you won't find anywhere else.

**Product Innovation** — An integral part of how we flex to your specs.

## Contents

|                           |                |
|---------------------------|----------------|
| Anion Standards .....     | 58-59          |
| Cation Standards .....    | 60             |
| Multi-Ion Standards.....  | 61             |
| Eluent Concentrates ..... | 61             |
| EPA Standards.....        | 62-64          |
| Custom IC Standards.....  | see pages 7-10 |

- ✓ **Traceable to NIST SRMs and lots**
- ✓ **Produced under ISO Guide 9001:2000**
- ✓ **Produced under ISO Guide 17025:2005**
- ✓ **Produced under ISO Guide 34:2000**
- ✓ **Assayed by validated Wet Chemical procedures**
- ✓ **Assayed by validated IC procedures**



1000 µg/mL

1000 µg/mL Anions

Custom anion standards are available upon request.

| Analyte  | Matrix                           | Starting Material                              | Volume           | Catalog #              |
|--|----------------------------------|--|------------------|------------------------|
| Acetate, C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> <sup>-</sup>   | H <sub>2</sub> O                 | Sodium acetate                                 | 125 mL<br>500 mL | ICOAC1-1<br>ICOAC1-5   |
| <b>NEW</b> Adipate, C <sub>6</sub> H <sub>8</sub> O <sub>4</sub>     | H <sub>2</sub> O                 | Adipic acid                                    | 125 mL<br>500 mL | ICADP1-1<br>ICADP1-5   |
| Benzoate, C <sub>6</sub> H <sub>5</sub> CO <sub>2</sub> <sup>-</sup> | H <sub>2</sub> O                 | Benzoic acid                                   | 125 mL<br>500 mL | ICBEN1-1<br>ICBEN1-5   |
| Bromate, BrO <sub>3</sub> <sup>-</sup>                               | H <sub>2</sub> O                 | KBrO <sub>3</sub>                              | 125 mL<br>500 mL | ICBRO31-1<br>ICBRO31-5 |
| Bromide, Br <sup>-</sup>   | H <sub>2</sub> O                 | KBr  | 125 mL<br>500 mL | ICBR1-1<br>ICBR1-5     |
| <b>NEW</b> Butyrate, C <sub>4</sub> H <sub>7</sub> O <sub>2</sub>    | H <sub>2</sub> O                 | Butyric Acid                                   | 125 mL<br>500 mL | ICBTR1-1<br>ICBTR1-5   |
| Carbonate, CO <sub>3</sub> <sup>-2</sup>                             | H <sub>2</sub> O                 | Na <sub>2</sub> CO <sub>3</sub>                | 125 mL<br>500 mL | ICCO31-1<br>ICCO31-5   |
| Chlorate, ClO <sub>3</sub> <sup>-</sup>                              | H <sub>2</sub> O                 | KClO <sub>3</sub>                              | 125 mL<br>500 mL | ICCLO31-1<br>ICCLO31-5 |
| Chloride, Cl <sup>-</sup>  | H <sub>2</sub> O                 | KCl  | 125 mL<br>500 mL | ICCL1-1<br>ICCL1-5     |
| Chlorite, ClO <sub>2</sub> <sup>-</sup>                              | H <sub>2</sub> O                 | NaClO <sub>2</sub>                             | 125 mL<br>500 mL | ICCLO21-1<br>ICCLO21-5 |
| Chromate, CrO <sub>4</sub> <sup>-2</sup>                             | H <sub>2</sub> O                 | NH <sub>4</sub> Cr <sub>2</sub> O <sub>7</sub> | 125 mL<br>500 mL | ICCRO41-1<br>ICCRO41-5 |
| Citrate, C <sub>6</sub> H <sub>5</sub> O <sub>7</sub> <sup>-3</sup>  | H <sub>2</sub> O                 | Citric Acid                                    | 125 mL<br>500 mL | ICCIT1-1<br>ICCIT1-5   |
| Fluoride, F <sup>-</sup>   | H <sub>2</sub> O                 | NaF  | 125 mL<br>500 mL | ICF1-1<br>ICF1-5       |
| Formate, HCO <sub>2</sub> <sup>-</sup>                               | H <sub>2</sub> O                 | Sodium Formate                                 | 125 mL<br>500 mL | ICHCO1-1<br>ICHCO1-5   |
| <b>NEW</b> Glutarate, C <sub>5</sub> H <sub>6</sub> O <sub>4</sub>   | H <sub>2</sub> O                 | Glutaric Acid                                  | 125 mL<br>500 mL | ICGTR1-1<br>ICGTR1-5   |
| Glycolate, C <sub>2</sub> H <sub>3</sub> O <sub>3</sub> <sup>-</sup> | H <sub>2</sub> O                 | Glycolic acid                                  | 125 mL<br>500 mL | ICGLY1-1<br>ICGLY1-5   |
| Iodide, I <sup>-</sup>   | H <sub>2</sub> O /<br>stabilizer | NH <sub>4</sub> I                              | 125 mL<br>500 mL | ICI1-1<br>ICI1-5       |
| Lactate, C <sub>3</sub> H <sub>5</sub> O <sub>3</sub> <sup>-</sup>   | H <sub>2</sub> O                 | Lactic acid                                    | 125 mL<br>500 mL | ICLCT1-1<br>ICLCT1-5   |
| Malate, C <sub>4</sub> H <sub>4</sub> O <sub>5</sub> <sup>-2</sup>   | H <sub>2</sub> O                 | Malic acid                                     | 125 mL<br>500 mL | ICMLA1-1<br>ICMLA1-5   |
| Maleate, C <sub>4</sub> H <sub>2</sub> O <sub>4</sub> <sup>-2</sup>  | H <sub>2</sub> O                 | Maleic acid                                    | 125 mL<br>500 mL | ICMLE1-1<br>ICMLE1-5   |
| <b>NEW</b> Malonate, C <sub>3</sub> H <sub>2</sub> O <sub>4</sub>    | H <sub>2</sub> O                 | Malonic Acid                                   | 125 mL<br>500 mL | ICMLO1-1<br>ICMLO1-5   |
| Methanesulfonate, CH <sub>3</sub> SO <sub>3</sub> <sup>-</sup>       | H <sub>2</sub> O                 | Methanesulfonic acid                           | 125 mL<br>500 mL | ICMSA1-1<br>ICMSA1-5   |
| Nitrate, NO <sub>3</sub> <sup>-</sup>                                | H <sub>2</sub> O                 | NaNO <sub>3</sub>                              | 125 mL<br>500 mL | ICNO31-1<br>ICNO31-5   |

**1000 µg/mL Anions** (continued)

Custom anion standards are available upon request.

**1000 µg/mL**

| Analyte  | Matrix           | Starting Material                              | Volume           | Catalog #              |
|--|------------------|--|------------------|------------------------|
| Nitrate as N   | H <sub>2</sub> O | NaNO <sub>3</sub>                              | 125 mL<br>500 mL | ICNNO31-1<br>ICNNO31-5 |
| Nitritotriacetate,<br>NC <sub>6</sub> H <sub>6</sub> O <sub>6</sub> <sup>-3</sup>      | H <sub>2</sub> O | Nitritotriacetic acid                          | 125 mL<br>500 mL | ICNTA1-1<br>ICNTA1-5   |
| Nitrite, NO <sub>2</sub> <sup>-</sup>  | H <sub>2</sub> O | NaNO <sub>2</sub>                              | 125 mL<br>500 mL | ICNO21-1<br>ICNO21-5   |
| Nitrite as N   | H <sub>2</sub> O | NaNO <sub>2</sub>                              | 125 mL<br>500 mL | ICNNO21-1<br>ICNNO21-5 |
| Oxalate, C <sub>2</sub> O <sub>4</sub> <sup>-2</sup>                                   | H <sub>2</sub> O | Sodium oxalate                                 | 125 mL<br>500 mL | ICOX1-1<br>ICOX1-5     |
| Perchlorate, ClO <sub>4</sub> <sup>-</sup>   | H <sub>2</sub> O | KClO <sub>4</sub>                              | 125 mL<br>500 mL | ICCLO41-1<br>ICCLO41-5 |
| Phosphate, PO <sub>4</sub> <sup>-3</sup>   | H <sub>2</sub> O | NH <sub>4</sub> H <sub>2</sub> PO <sub>4</sub> | 125 mL<br>500 mL | ICPO41-1<br>ICPO41-5   |
| Phosphate as P   | H <sub>2</sub> O | NH <sub>4</sub> H <sub>2</sub> PO <sub>4</sub> | 125 mL<br>500 mL | ICPPO41-1<br>ICPPO41-5 |
| Phthalate, C <sub>6</sub> H <sub>4</sub> (CO <sub>2</sub> ) <sub>2</sub> <sup>-2</sup> | H <sub>2</sub> O | Potassium hydrogen phthalate                   | 125 mL<br>500 mL | ICKHP1-1<br>ICKHP1-5   |
| Propionate, C <sub>2</sub> H <sub>5</sub> CO <sub>2</sub> <sup>-</sup>                 | H <sub>2</sub> O | Sodium propionate                              | 125 mL<br>500 mL | ICOPR1-1<br>ICOPR1-5   |
| Succinate, C <sub>4</sub> H <sub>4</sub> O <sub>4</sub> <sup>-2</sup>                  | H <sub>2</sub> O | Succinic acid                                  | 125 mL<br>500 mL | ICSCC1-1<br>ICSCC1-5   |
| Sulfate, SO <sub>4</sub> <sup>-2</sup>   | H <sub>2</sub> O | K <sub>2</sub> SO <sub>4</sub>                 | 125 mL<br>500 mL | ICSO41-1<br>ICSO41-5   |
| Tartrate, C <sub>4</sub> H <sub>4</sub> O <sub>6</sub> <sup>-2</sup>                   | H <sub>2</sub> O | Tartaric acid                                  | 125 mL<br>500 mL | ICTRTR1-1<br>ICTRTR1-5 |
| Thiocyanate, SCN <sup>-</sup>  | H <sub>2</sub> O | KSCN   | 125 mL<br>500 mL | ICSCN1-1<br>ICSCN1-5   |
| Thiosulfate, S <sub>2</sub> O <sub>3</sub> <sup>-2</sup>                               | H <sub>2</sub> O | Sodium thiosulfate                             | 125 mL<br>500 mL | ICS2O31-1<br>ICS2O31-5 |

**Devoted...**

We love Inorganic Ventures. Every time we need something, the staff that we deal with is so helpful and kind. It really seems that we are their most important customer at that time.

Randi Richey  
Huntsville, AL

*"We work hard to get your orders out on time!"*

**Jeanette Eason**  
Packaging Technician





## 1000 µg/mL Cation

Custom cation standards are available upon request.

# 1000 µg/mL

| Analyte  | Matrix               | Starting Material                | Volume           | Catalog #              |
|--|----------------------|----------------------------------|------------------|------------------------|
| 3-Methoxypropylamine,<br>$\text{CH}_3\text{O}(\text{CH}_2)_3\text{NH}_2$ | HCl                  | 3-Methoxypropylamine             | 125 mL           | ICMPA1-1               |
|  |                      |                                  | 500 mL           | ICMPA1-5               |
| Ammonium, $\text{NH}_4^+$  | $\text{H}_2\text{O}$ | $\text{NH}_4\text{Cl}$           | 125 mL           | ICNH41-1               |
|  |                      |                                  | 500 mL           | ICNH41-5               |
| Ammonium as N  | $\text{H}_2\text{O}$ | $\text{NH}_4\text{Cl}$           | 125 mL<br>500 mL | ICNNH41-1<br>ICNNH41-5 |
| Barium, $\text{Ba}^{+2}$   | $\text{HNO}_3$       | $\text{Ba}(\text{NO}_3)_2$       | 125 mL           | ICBA1-1                |
|  |                      |                                  | 500 mL           | ICBA1-5                |
| Calcium, $\text{Ca}^{+2}$  | $\text{HNO}_3$       | CaO                              | 125 mL           | ICCA1-1                |
|  |                      |                                  | 500 mL           | ICCA1-5                |
| Cesium, $\text{Cs}^+$  | $\text{HNO}_3$       | $\text{CsNO}_3$                  | 125 mL           | ICCS1-1                |
|  |                      |                                  | 500 mL           | ICCS1-5                |
| Diethanolamine,<br>$(\text{HOCH}_2\text{CH}_2)_2\text{NH}$               | $\text{H}_2\text{O}$ | Diethanolamine                   | 125 mL           | ICDEA1-1               |
|  |                      |                                  | 500 mL           | ICDEA1-5               |
| Dimethylamine,<br>$\text{NH}(\text{CH}_3)_2$                             | HCl                  | Dimethylamine                    | 125 mL           | ICDMA1-1               |
|  |                      |                                  | 500 mL           | ICDMA1-5               |
| Lithium, $\text{Li}^+$   | $\text{HNO}_3$       | $\text{Li}_2\text{CO}_3$         | 125 mL           | ICLI1-1                |
|  |                      |                                  | 500 mL           | ICLI1-5                |
| Magnesium, $\text{Mg}^{+2}$  | $\text{HNO}_3$       | Mg metal                         | 125 mL           | ICMG1-1                |
|  |                      |                                  | 500 mL           | ICMG1-5                |
| Monoethanolamine,<br>$\text{HOCH}_2\text{CH}_2\text{NH}_2$               | $\text{H}_2\text{O}$ | Monoethanolamine                 | 125 mL           | ICMEA1-1               |
|  |                      |                                  | 500 mL           | ICMEA1-5               |
| Monomethylamine,<br>$\text{NH}_2\text{CH}_3$                             | HCl                  | Monomethylamine                  | 125 mL           | ICMMA1-1               |
|  |                      |                                  | 500 mL           | ICMMA1-5               |
| Potassium, $\text{K}^+$  | $\text{HNO}_3$       | $\text{KNO}_3$                   | 125 mL           | ICK1-1                 |
|  |                      |                                  | 500 mL           | ICK1-5                 |
| Rubidium, $\text{Rb}^+$  | $\text{HNO}_3$       | $\text{RbNO}_3$                  | 125 mL           | ICRB1-1                |
|  |                      |                                  | 500 mL           | ICRB1-5                |
| Sodium, $\text{Na}^+$  | $\text{HNO}_3$       | $\text{Na}_2\text{CO}_3$         | 125 mL           | ICNA1-1                |
|  |                      |                                  | 500 mL           | ICNA1-5                |
| Strontium, $\text{Sr}^{+2}$  | $\text{HNO}_3$       | $\text{SrCO}_3$                  | 125 mL           | ICSR1-1                |
|  |                      |                                  | 500 mL           | ICSR1-5                |
| Tetramethylammonium,<br>$\text{N}^+(\text{CH}_3)_4$                      | $\text{H}_2\text{O}$ | Tetramethylammonium<br>hydroxide | 125 mL           | ICTMAH1-1              |
|  |                      |                                  | 500 mL           | ICTMAH1-5              |
| Triethanolamine,<br>$(\text{HOCH}_2\text{CH}_2)_3\text{N}$               | $\text{H}_2\text{O}$ | Triethanolamine                  | 125 mL           | ICTEA1-1               |
|  |                      |                                  | 500 mL           | ICTEA1-5               |
| Triethylamine,<br>$(\text{CH}_3\text{CH}_2)_3\text{N}$                   | HCl                  | Triethylamine                    | 125 mL           | ICTA1-1                |
|  |                      |                                  | 500 mL           | ICTA1-5                |
| Trimethylamine,<br>$(\text{CH}_3)_3\text{N}$                             | HCl                  | Trimethylamine                   | 125 mL           | ICTMA1-1               |
|  |                      |                                  | 500 mL           | ICTMA1-5               |

Custom multi-ion standards are available upon request.

### Anion Calibration Standard

IC-FAS-1A

Volume 125 mL

Matrix H<sub>2</sub>O

| Analyte                      | µg/mL | Analyte                       | µg/mL |
|------------------------------|-------|-------------------------------|-------|
| Br <sup>-</sup>              | 100   | NO <sub>2</sub> <sup>-</sup>  | 100   |
| Cl <sup>-</sup>              | 30    | PO <sub>4</sub> <sup>-3</sup> | 150   |
| F <sup>-</sup>               | 20    | SO <sub>4</sub> <sup>-2</sup> | 150   |
| NO <sub>3</sub> <sup>-</sup> | 100   |                               |       |

Used for daily calibration.

### Cation Calibration Standard 2

IV-STOCK-7

Volume 125 mL

Matrix HNO<sub>3</sub>

**NEW**

| Analyte          | µg/mL | Analyte                      | µg/mL |
|------------------|-------|------------------------------|-------|
| Ba <sup>+2</sup> | 100   | Mn <sup>+2</sup>             | 100   |
| Ca <sup>+2</sup> | 100   | Na <sup>+</sup>              | 100   |
| K <sup>+</sup>   | 100   | NH <sub>4</sub> <sup>+</sup> | 100   |
| Li <sup>+</sup>  | 100   | Sr <sup>+2</sup>             | 100   |
| Mg <sup>+2</sup> | 100   |                              |       |

Used for daily calibration.

### Cation Calibration Standard 1

IC-SCS1-1

\$105.00

Volume 125 mL

Matrix HNO<sub>3</sub>

| Analyte          | µg/mL | Analyte                      | µg/mL |
|------------------|-------|------------------------------|-------|
| Ca <sup>+2</sup> | 1000  | Mg <sup>+2</sup>             | 200   |
| K <sup>+</sup>   | 200   | Na <sup>+</sup>              | 200   |
| Li <sup>+</sup>  | 50    | NH <sub>4</sub> <sup>+</sup> | 400   |

Used for daily calibration.

## ELUENT CONCENTRATES

Custom eluent concentrates are available upon request.

### 0.18 M Sodium Carbonate / 0.17 M Sodium Bicarbonate

ELUENT1817-1 100 mL

ELUENT1817-5 500 mL

Matrix H<sub>2</sub>O

Dilution 1:100

For preparation of 1.8 mM CO<sub>3</sub><sup>-2</sup> / 1.7 mM HCO<sub>3</sub><sup>-</sup> eluent.

### 0.5 M Sodium Carbonate

CARB-1 100 mL

CARB-5 500 mL

Matrix H<sub>2</sub>O

Dilution 1:100

For preparation of various CO<sub>3</sub><sup>-2</sup> / HCO<sub>3</sub><sup>-</sup> eluents.

### 0.35 M Sodium Carbonate / 0.10 M Sodium Bicarbonate

ELUENT3510-1 100 mL

ELUENT3510-5 500 mL

Matrix H<sub>2</sub>O

Dilution 1:100

For preparation of 3.5 mM CO<sub>3</sub><sup>-2</sup> / 1.0 mM HCO<sub>3</sub><sup>-</sup> eluent.

### 1.8 M Methanesulfonic Acid

MSAELUENT-1 100 mL

MSAELUENT-5 500 mL

Matrix H<sub>2</sub>O

Dilution 1:100

For preparation of 18 mM CH<sub>3</sub>SO<sub>3</sub>H eluent for analyzing cations.

### 0.5 M Sodium Bicarbonate

BICARB-1 100 mL

BICARB-5 500 mL

Matrix H<sub>2</sub>O

Dilution 1:100

For preparation of various CO<sub>3</sub><sup>-2</sup> / HCO<sub>3</sub><sup>-</sup> eluents.



## Method 300.0 & 300.1

Custom EPA standards are available upon request.

### 300.0 Rev. 2.1 Part A

#### 0.18 M Sodium Carbonate / 0.17 M Sodium Bicarbonate

ELUENT1817-1     100 mL  
 ELUENT1817-5     500 mL  
 Matrix            H<sub>2</sub>O  
 Dilution          1:100

For preparation of 1.8 mM CO<sub>3</sub><sup>-2</sup> / 1.7 mM HCO<sub>3</sub><sup>-</sup> eluent.

#### Calibration Standard

300-CAL-A  
 Volume          125 mL  
 Matrix            H<sub>2</sub>O  
 Dilution          1:10 to 1:100

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 100   | Nitrite as N                  | 30    |
| Cl <sup>-</sup> | 30    | Nitrate as N                  | 25    |
| F <sup>-</sup>  | 20    | SO <sub>4</sub> <sup>-2</sup> | 150   |
| Phosphate as P  | 50    |                               |       |

#### Laboratory Fortification Stock Standard

300-LFS-A  
 Volume          125 mL  
 Matrix            H<sub>2</sub>O  
 Dilution          1:100 to 1:1000

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 1000  | Nitrite as N                  | 300   |
| Cl <sup>-</sup> | 300   | Nitrate as N                  | 300   |
| F <sup>-</sup>  | 200   | SO <sub>4</sub> <sup>-2</sup> | 1500  |
| Phosphate as P  | 500   |                               |       |

This standard is used to prepare the Laboratory Fortified Blank and the Laboratory Fortified Sample Matrix.

#### QC Standard / Instrument Performance Check<sup>†</sup>

QCP-QCS-5  
 Volume          125 mL  
 Matrix            H<sub>2</sub>O  
 Dilution          1:10 to 1:100

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 50    | Nitrite as N                  | 15    |
| Cl <sup>-</sup> | 15    | Nitrate as N                  | 10    |
| F <sup>-</sup>  | 10    | SO <sub>4</sub> <sup>-2</sup> | 75    |
| Phosphate as P  | 25    |                               |       |

Can be used to prepare the QC Sample or the IPC Solution.  
<sup>†</sup>Manufactured from in-house Second Source concentrates.



*"Here at Inorganic Ventures, we set the standards and our standards are set for excellence."*

**Angela Sinclair**  
Product Documentation

## Method 300.0 & 300.1 (continued)

Custom EPA standards are available upon request.

### 300.1 Part A

#### 0.18 M Sodium Carbonate / 0.17 M Sodium Bicarbonate

|              |                  |
|--------------|------------------|
| ELUENT1817-1 | 100 mL           |
| ELUENT1817-5 | 500 mL           |
| Matrix       | H <sub>2</sub> O |
| Dilution     | 1:100            |

For preparation of 1.8 mM CO<sub>3</sub><sup>2-</sup> / 1.7 mM HCO<sub>3</sub><sup>-</sup> eluent.

#### Calibration Standard

##### 300-CAL-A

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:10 to 1:100    |

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 100   | Nitrite as N                  | 30    |
| Cl <sup>-</sup> | 30    | Nitrate as N                  | 25    |
| F <sup>-</sup>  | 20    | SO <sub>4</sub> <sup>2-</sup> | 150   |
| Phosphate as P  | 50    |                               |       |

#### Dichloroacetate Standard

|           |                  |
|-----------|------------------|
| ICDCA-S-1 | 125 mL           |
| ICDCA-S-5 | 500 mL           |
| Matrix    | H <sub>2</sub> O |

| Analyte   | µg/mL |
|---|-------|
| Cl <sub>2</sub> HC <sub>2</sub> O <sub>2</sub> <sup>-</sup> | 500   |

For use as a surrogate analyte.

#### Laboratory Fortification Stock Standard

##### 300-LFS-A

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100 to 1:1000  |

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 1000  | Nitrite as N                  | 300   |
| Cl <sup>-</sup> | 300   | Nitrate as N                  | 300   |
| F <sup>-</sup>  | 200   | SO <sub>4</sub> <sup>2-</sup> | 1500  |
| Phosphate as P  | 500   |                               |       |

This standard is used to prepare the Laboratory Fortified Blank and the Laboratory Fortified Sample Matrix.

#### QC Standard / Instrument Performance Check†

##### QCP-QCS-5

|          |                  |
|----------|------------------|
| Volume   | 125 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:10 to 1:100    |

| Analyte         | µg/mL | Analyte                       | µg/mL |
|-----------------|-------|-------------------------------|-------|
| Br <sup>-</sup> | 50    | Nitrite as N                  | 15    |
| Cl <sup>-</sup> | 15    | Nitrate as N                  | 10    |
| F <sup>-</sup>  | 10    | SO <sub>4</sub> <sup>2-</sup> | 75    |
| Phosphate as P  | 25    |                               |       |

Can be used to prepare the QC Sample or the IPC Solution.

†Manufactured from in-house Second Source concentrates.

## Reliable...

We are currently using your cation and anion standards for IC analysis. The solutions give very reliable calibration. We are going to use more of your ion standards in the future.

Jianguo Chen  
Sunnyvale, CA

## Method 300.0 & 300.1 (continued)

Custom EPA standards are available upon request.

### 300.1 Part B

#### Bromate

ICBRO31-1  
Volume 125 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**BrO<sub>3</sub><sup>-</sup>** 1000

#### Bromide

ICBR1-1  
Volume 125 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**Br<sup>-</sup>** 1000

#### Chlorate

ICCLO31-1  
Volume 125 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**ClO<sub>3</sub><sup>-</sup>** 1000

#### Chlorite

ICCLO21-1  
Volume 125 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**ClO<sub>2</sub><sup>-</sup>** 1000

NOTE: Contains less than 10ppm ClO<sub>3</sub><sup>-</sup>.

#### Dichloroacetate Standard

ICDCA-S-1 125 mL  
ICDCA-S-5 500 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**Cl<sub>2</sub>HC<sub>2</sub>O<sub>2</sub><sup>-</sup>** 500

For use as a surrogate analyte.

## Method 314.0

Custom EPA standards are available upon request.

#### 1400 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON1400-25  
Volume 125 mL  
Matrix H<sub>2</sub>O

#### Perchlorate

ICCLO41-1  
Volume 125 mL  
Matrix H<sub>2</sub>O

**Analyte**  $\mu\text{g/mL}$

**ClO<sub>4</sub><sup>-</sup>** 1000

#### Mixed Anion Stock Solution

314-ANION-STOCK  
Volume 125 mL  
Matrix H<sub>2</sub>O

| Analyte                       | $\mu\text{g/mL}$ | Analyte                       | $\mu\text{g/mL}$ |
|-------------------------------|------------------|-------------------------------|------------------|
| Cl <sup>-</sup>               | 25,000           | SO <sub>4</sub> <sup>-2</sup> | 25,000           |
| CO <sub>3</sub> <sup>-2</sup> | 25,000           |                               |                  |

NOTE: This is not a CRM. This is the anion stock solution used to determine the MCT (Matrix Conductivity Threshold) for Method 314.0.

# ATOMIC ABSORPTION



If Atomic Absorption is your instrument of choice, we think you'll appreciate our improved line of AA standards. We've more than doubled our previous selection of analytical elements. And if you still can't find what you need, just ask. Customization is our specialty.

**Improved Selection** — One more way that we flex to your specs.

## Contents

|   |                |
|---|----------------|
| Single-Element Standards .....              | 66-68          |
| Modifiers, Buffers & Releasing Agents ..... | 69             |
| EPA Standards .....                         | 70             |
| Custom AA Solutions .....                   | see pages 7-10 |

- ✓ **Traceable to NIST SRMs and lots**
- ✓ **Produced under ISO Guide 9001:2000**
- ✓ **Assayed by validated procedures**



ATOMIC ABSORPTION  
SINGLE-ELEMENT STANDARDS



**1000 µg/mL Standards**

Custom atomic absorption standards are available upon request.

**1000 µg/mL**

| Analyte        | Matrix                                | Starting Material   | Volume | Catalog # |
|----------------|---------------------------------------|---|--------|-----------|
| Aluminum, Al   | HNO <sub>3</sub>                      | Al metal  | 125 mL | AAAL1-1   |
|                |                                       |   | 500 mL | AAAL1-5   |
| Antimony, Sb   | HNO <sub>3</sub> /<br>Tartaric Acid   | Sb metal  | 125 mL | AASB1-1   |
|                |                                       |   | 500 mL | AASB1-5   |
| Arsenic, As    | HNO <sub>3</sub>                      | As metal  | 125 mL | AAAS1-1   |
|                |                                       |   | 500 mL | AAAS1-5   |
| Barium, Ba     | HNO <sub>3</sub>                      | Ba(NO <sub>3</sub> ) <sub>2</sub>   | 125 mL | AABA1-1   |
|                |                                       |   | 500 mL | AABA1-5   |
| Beryllium, Be  | HNO <sub>3</sub>                      | Be <sub>4</sub> O(C <sub>2</sub> H <sub>3</sub> O <sub>2</sub> ) <sub>6</sub> | 125 mL | AABE1-1   |
|                |                                       |   | 500 mL | AABE1-5   |
| Bismuth, Bi    | HNO <sub>3</sub>                      | Bi metal  | 125 mL | AABI1-1   |
|                |                                       |   | 500 mL | AABI1-5   |
| Boron, B       | H <sub>2</sub> O                      | H <sub>3</sub> BO <sub>3</sub>  | 125 mL | AAB1-1    |
|                |                                       |   | 500 mL | AAB1-5    |
| Cadmium, Cd    | HNO <sub>3</sub>                      | Cd metal  | 125 mL | AACD1-1   |
|                |                                       |   | 500 mL | AACD1-5   |
| Calcium, Ca    | HNO <sub>3</sub>                      | CaO   | 125 mL | AACA1-1   |
|                |                                       |   | 500 mL | AACA1-5   |
| Cerium, Ce     | HNO <sub>3</sub>                      | CeO <sub>2</sub>  | 125 mL | AACE1-1   |
|                |                                       |   | 500 mL | AACE1-5   |
| Cesium, Cs     | HNO <sub>3</sub>                      | CsNO <sub>3</sub>   | 125 mL | AACS1-1   |
|                |                                       |   | 500 mL | AACS1-5   |
| Chromium, Cr   | HNO <sub>3</sub>                      | Cr metal  | 125 mL | AACR1-1   |
|                |                                       |   | 500 mL | AACR1-5   |
| Cobalt, Co     | HNO <sub>3</sub>                      | Co metal  | 125 mL | AACO1-1   |
|                |                                       |   | 500 mL | AACO1-5   |
| Copper, Cu     | HNO <sub>3</sub>                      | Cu metal  | 125 mL | AACU1-1   |
|                |                                       |   | 500 mL | AACU1-5   |
| Dysprosium, Dy | HNO <sub>3</sub>                      | Dy <sub>2</sub> O <sub>3</sub>  | 125 mL | AADY1-1   |
|                |                                       |   | 500 mL | AADY1-5   |
| Erbium, Er     | HNO <sub>3</sub>                      | Er <sub>2</sub> O <sub>3</sub>  | 125 mL | AAER1-1   |
|                |                                       |   | 500 mL | AAER1-5   |
| Europium, Eu   | HNO <sub>3</sub>                      | Eu <sub>2</sub> O <sub>3</sub>  | 125 mL | AAEU1-1   |
|                |                                       |   | 500 mL | AAEU1-5   |
| Gadolinium, Gd | HNO <sub>3</sub>                      | Gd <sub>2</sub> O <sub>3</sub>  | 125 mL | AAGD1-1   |
|                |                                       |   | 500 mL | AAGD1-5   |
| Gallium, Ga    | HNO <sub>3</sub>                      | Ga metal  | 125 mL | AAGA1-1   |
|                |                                       |   | 500 mL | AAGA1-5   |
| Germanium, Ge  | H <sub>2</sub> O/HNO <sub>3</sub> /HF | Ge metal  | 125 mL | AAGE1-1   |
|                |                                       |   | 500 mL | AAGE1-5   |
| Gold, Au       | HCl                                   | AuCl <sub>3</sub>   | 125 mL | AAAU1-1   |
|                |                                       |   | 500 mL | AAAU1-5   |
| Hafnium, Hf    | H <sub>2</sub> O/HNO <sub>3</sub> /HF | HfO <sub>2</sub>  | 125 mL | AAHF1-1   |
|                |                                       |   | 500 mL | AAHF1-5   |
| Holmium, Ho    | HNO <sub>3</sub>                      | Ho <sub>2</sub> O <sub>3</sub>  | 125 mL | AAHO1-1   |
|                |                                       |   | 500 mL | AAHO1-5   |
| Indium, In     | HNO <sub>3</sub>                      | In metal  | 125 mL | AAIN1-1   |
|                |                                       |   | 500 mL | AAIN1-5   |

**1000 µg/mL Standards** (continued)

Custom atomic absorption standards are available upon request.

**1000 µg/mL**

| Analyte          | Matrix                                | Starting Material                                | Volume | Catalog # |
|------------------|---------------------------------------|--|--------|-----------|
| Iridium, Ir      | HCl                                   | IrCl <sub>3</sub>                                | 125 mL | AAIR1-1   |
|                  |                                       |  | 500 mL | AAIR1-5   |
| Iron, Fe         | HNO <sub>3</sub>                      | Fe metal   | 125 mL | AAFE1-1   |
|                  |                                       |  | 500 mL | AAFE1-5   |
| Lanthanum, La    | HNO <sub>3</sub>                      | La <sub>2</sub> O <sub>3</sub>                   | 125 mL | AALA1-1   |
|                  |                                       |  | 500 mL | AALA1-5   |
| Lead, Pb         | HNO <sub>3</sub>                      | Pb(NO <sub>3</sub> ) <sub>2</sub>                | 125 mL | AAPB1-1   |
|                  |                                       |  | 500 mL | AAPB1-5   |
| Lithium, Li      | HNO <sub>3</sub>                      | Li <sub>2</sub> CO <sub>3</sub>                  | 125 mL | AALI1-1   |
|                  |                                       |  | 500 mL | AALI1-5   |
| Lutetium, Lu     | HNO <sub>3</sub>                      | Lu <sub>2</sub> O <sub>3</sub>                   | 125 mL | AALU1-1   |
|                  |                                       |  | 500 mL | AALU1-5   |
| Magnesium, Mg    | HNO <sub>3</sub>                      | Mg metal   | 125 mL | AAMG1-1   |
|                  |                                       |  | 500 mL | AAMG1-5   |
| Manganese, Mn    | HNO <sub>3</sub>                      | Mn metal   | 125 mL | AAMN1-1   |
|                  |                                       |  | 500 mL | AAMN1-5   |
| Mercury, Hg      | HNO <sub>3</sub>                      | Hg metal   | 125 mL | AAHG1-1   |
|                  |                                       |  | 500 mL | AAHG1-5   |
| Molybdenum, Mo   | H <sub>2</sub> O/NH <sub>4</sub> OH   | (NH <sub>4</sub> ) <sub>2</sub> MoO <sub>4</sub> | 125 mL | AAMO1-1   |
|                  |                                       |  | 500 mL | AAMO1-5   |
| Neodymium, Nd    | HNO <sub>3</sub>                      | Nd <sub>2</sub> O <sub>3</sub>                   | 125 mL | AAND1-1   |
|                  |                                       |  | 500 mL | AAND1-5   |
| Nickel, Ni       | HNO <sub>3</sub>                      | Ni metal   | 125 mL | AANI1-1   |
|                  |                                       |  | 500 mL | AANI1-5   |
| Niobium, Nb      | H <sub>2</sub> O/HNO <sub>3</sub> /HF | Nb metal   | 125 mL | AANB1-1   |
|                  |                                       |  | 500 mL | AANB1-5   |
| Palladium, Pd    | HCl                                   | Pd(NO <sub>3</sub> ) <sub>2</sub>                | 125 mL | AAPD1-1   |
|                  |                                       |  | 500 mL | AAPD1-5   |
| Phosphorus, P    | H <sub>2</sub> O                      | H <sub>3</sub> PO <sub>4</sub>                   | 125 mL | AAP1-1    |
|                  |                                       |  | 500 mL | AAP1-5    |
| Platinum, Pt     | HCl                                   | Pt metal   | 125 mL | AAPT1-1   |
|                  |                                       |  | 500 mL | AAPT1-5   |
| Potassium, K     | HNO <sub>3</sub>                      | KNO <sub>3</sub>                                 | 125 mL | AAK1-1    |
|                  |                                       |  | 500 mL | AAK1-5    |
| Praseodymium, Pr | HNO <sub>3</sub>                      | Pr <sub>6</sub> O <sub>11</sub>                  | 125 mL | AAPR1-1   |
|                  |                                       |  | 500 mL | AAPR1-5   |
| Rhenium, Re      | HNO <sub>3</sub>                      | Re metal   | 125 mL | AARE1-1   |
|                  |                                       |  | 500 mL | AARE1-5   |
| Rhodium, Rh      | HCl                                   | RhCl <sub>3</sub>                                | 125 mL | AARH1-1   |
|                  |                                       |  | 500 mL | AARH1-5   |
| Rubidium, Rb     | HNO <sub>3</sub>                      | RbNO <sub>3</sub>                                | 125 mL | AARB1-1   |
|                  |                                       |  | 500 mL | AARB1-5   |
| Ruthenium, Ru    | HCl                                   | NH <sub>4</sub> RuCl <sub>6</sub>                | 125 mL | AARU1-1   |
|                  |                                       |  | 500 mL | AARU1-5   |
| Samarium, Sm     | HNO <sub>3</sub>                      | Sm <sub>2</sub> O <sub>3</sub>                   | 125 mL | AASM1-1   |
|                  |                                       |  | 500 mL | AASM1-5   |
| Scandium, Sc     | HNO <sub>3</sub>                      | Sc <sub>2</sub> O <sub>3</sub>                   | 125 mL | AASC1-1   |
|                  |                                       |  | 500 mL | AASC1-5   |

ATOMIC ABSORPTION  
SINGLE-ELEMENT STANDARDS



**1000 µg/mL Standards** (continued)

Custom atomic absorption standards are available upon request.

1000 µg/mL

| Analyte       | Matrix                                 | Starting Material                                    | Volume | Catalog # |
|---------------|--|--|--------|-----------|
| Selenium, Se  | HNO <sub>3</sub>                       | Se metal   | 125 mL | AASE1-1   |
|               |  |  | 500 mL | AASE1-5   |
| Silicon, Si   | H <sub>2</sub> O/HNO <sub>3</sub> /HF  | SiO <sub>2</sub>                                     | 125 mL | AASI1-1   |
|               |  |  | 500 mL | AASI1-5   |
| Silver, Ag    | HNO <sub>3</sub>                       | Ag metal   | 125 mL | AAAG1-1   |
|               |  |  | 500 mL | AAAG1-5   |
| Sodium, Na    | HNO <sub>3</sub>                       | Na <sub>2</sub> CO <sub>3</sub>                      | 125 mL | AANA1-1   |
|               |  |  | 500 mL | AANA1-5   |
| Strontium, Sr | HNO <sub>3</sub>                       | SrCO <sub>3</sub>                                    | 125 mL | AASR1-1   |
|               |  |  | 500 mL | AASR1-5   |
| Sulfur, S     | H <sub>2</sub> O                       | H <sub>2</sub> SO <sub>4</sub>                       | 125 mL | AAS1-1    |
|               |  |  | 500 mL | AAS1-5    |
| Tantalum, Ta  | HNO <sub>3</sub> /HF                   | Ta metal   | 125 mL | AATA1-1   |
|               |  |  | 500 mL | AATA1-5   |
| Tellurium, Te | HCl                                    | Te metal   | 125 mL | AATE1-1   |
|               |  |  | 500 mL | AATE1-5   |
| Terbium, Tb   | HNO <sub>3</sub>                       | Tb <sub>4</sub> O <sub>7</sub>                       | 125 mL | AATB1-1   |
|               |  |  | 500 mL | AATB1-5   |
| Thallium, Tl  | HNO <sub>3</sub>                       | TlNO <sub>3</sub>                                    | 125 mL | AATL1-1   |
|               |  |  | 500 mL | AATL1-5   |
| Thorium, Th   | HNO <sub>3</sub>                       | Th(NO <sub>3</sub> ) <sub>4</sub> ·xH <sub>2</sub> O | 125 mL | AATH1-1   |
|               |  |  | 500 mL | AATH1-5   |
| Thulium, Tm   | HNO <sub>3</sub>                       | Tm <sub>2</sub> O <sub>3</sub>                       | 125 mL | AATM1-1   |
|               |  |  | 500 mL | AATM1-5   |
| Tin, Sn       | H <sub>2</sub> O/ HNO <sub>3</sub> /HF | Sn metal   | 125 mL | AASN1-1   |
|               |  |  | 500 mL | AASN1-5   |
| Titanium, Ti  | HNO <sub>3</sub> /HF                   | Ti metal   | 125 mL | AATI1-1   |
|               |  |  | 500 mL | AATI1-5   |
| Tungsten, W   | HNO <sub>3</sub> /HF                   | W metal  | 125 mL | AAW1-1    |
|               |  |  | 500 mL | AAW1-5    |
| Uranium, U    | HNO <sub>3</sub>                       | UO <sub>2</sub> (NO <sub>3</sub> ) <sub>2</sub>      | 125 mL | AAU1-1    |
|               |  |  | 500 mL | AAU1-5    |
| Vanadium, V   | HNO <sub>3</sub>                       | V <sub>2</sub> O <sub>5</sub>                        | 125 mL | AAV1-1    |
|               |  |  | 500 mL | AAV1-5    |
| Ytterbium, Yb | HNO <sub>3</sub>                       | Yb <sub>2</sub> O <sub>3</sub>                       | 125 mL | AAYB1-1   |
|               |  |  | 500 mL | AAYB1-5   |
| Yttrium, Y    | HNO <sub>3</sub>                       | Y <sub>2</sub> O <sub>3</sub>                        | 125 mL | AAAY1-1   |
|               |  |  | 500 mL | AAAY1-5   |
| Zinc, Zn      | HNO <sub>3</sub>                       | Zn metal   | 125 mL | AAZN1-1   |
|               |  |  | 500 mL | AAZN1-5   |
| Zirconium, Zr | H <sub>2</sub> O/HF                    | ZrO <sub>2</sub>                                     | 125 mL | AAZR1-1   |
|               |  |  | 500 mL | AAZR1-5   |

Custom modifiers, buffers and releasing agents are available upon request.

**0.3% Palladium / 0.2% Magnesium Modifier**

MM-PDMG-32  
Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte                           | µg/mL | Analyte | µg/mL |
|-----------------------------------|-------|---------|-------|
| Mg(NO <sub>3</sub> ) <sub>2</sub> | 2000  | Pd      | 3000  |

**1% Palladium Modifier**

MM-PD-10  
Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL  |
|---------|--------|
| Pd      | 10,000 |

**0.5% Palladium Modifier**

MM-PD-5  
Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL |
|---------|-------|
| Pd      | 5000  |

**2% Lithium Ionization Buffer**

LINB2-5  
Volume 500 mL  
Matrix HNO<sub>3</sub>

| Analyte | µg/mL  |
|---------|--------|
| Li      | 20,000 |

**1% Lanthanum Releasing Agent**

LACB1-5  
Volume 500 mL  
Matrix HCl

| Analyte | µg/mL  |
|---------|--------|
| La      | 10,000 |

**4% Phosphate Modifier**

MM-P-40  
Volume 125 mL  
Matrix H<sub>2</sub>O

| Analyte  | µg/mL  |
|--|--------|
| NH <sub>4</sub> H <sub>2</sub> PO <sub>4</sub> | 40,000 |

**1% Magnesium Nitrate Modifier**

MM-MG-10  
Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte                           | µg/mL  |
|-----------------------------------|--------|
| Mg(NO <sub>3</sub> ) <sub>2</sub> | 10,000 |

MULTI-ELEMENT STANDARDS

Custom modifiers, buffers and releasing agents are available upon request.

**GFAA Calibration Standard**

IV-STOCK-18 **NEW**  
Volume 125 mL  
Matrix HNO<sub>3</sub>

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Ag               | 10    | Cu      | 50    |
| Al               | 100   | Fe      | 20    |
| As               | 100   | Mn      | 20    |
| Ba               | 50    | Ni      | 50    |
| Be               | 5     | Pb      | 100   |
| Cd               | 5     | Sb      | 100   |
| Co               | 50    | Se      | 100   |
| Cr <sup>+3</sup> | 20    | Tl      | 100   |

**AA Calibration Standard**

IV-STOCK-25 **NEW**  
Volume 500 mL  
Matrix HNO<sub>3</sub>

| Analyte          | µg/mL | Analyte | µg/mL |
|------------------|-------|---------|-------|
| Cr <sup>+3</sup> | 3     | Ni      | 10    |



## Toxicity Characteristic Leachate Procedure (TCLP)

Custom EPA standards are available upon request.

### TCLP Hg Standard

TCLP-AA-HG

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution As required

| Analyte | µg/mL |
|---------|-------|
| Hg      | 20    |

### TCLP Standard

TCLP-1REV

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:5

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| Ag      | 25    | Cr      | 25    |
| As      | 25    | Pb      | 25    |
| Ba      | 500   | Se      | 5     |
| Cd      | 5     |         |       |

## CLP Graphite Furnace Standards

Custom EPA standards are available upon request.

### Analytical Spiking Standard

CLPF-ASPK-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:10

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 20    | Sb      | 120   |
| Cd      | 10    | Se      | 10    |
| Pb      | 20    | Tl      | 20    |

### CCV / ICV Standard 4<sup>†</sup>

QCP-CICV-4

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:50

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 25    | Sb      | 50    |
| Cd      | 5     | Se      | 50    |
| Pb      | 25    | Tl      | 25    |

### Calibration Standard

CLPF-CAL-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:100

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 50    | Sb      | 100   |
| Cd      | 10    | Se      | 100   |
| Pb      | 50    | Tl      | 50    |

### Predigestion Spiking Standard

CLPF-PSPK-1

Volume 125 mL  
Matrix HNO<sub>3</sub>  
Dilution 1:1000

| Analyte | µg/mL | Analyte | µg/mL |
|---------|-------|---------|-------|
| As      | 40    | Sb      | 100   |
| Cd      | 5     | Se      | 10    |
| Pb      | 20    | Tl      | 50    |

<sup>†</sup>Manufactured from in-house Second Source concentrates.

## Unquestionable...

Inorganic Ventures always has what I need for Atomic Absorption and ICP. Their service is always spot-on and the integrity of their standards is unquestionable. Thanks for doing the very best.

*John Thiel  
Sparks, NV*



Should you ever have a problem with any standard, Water QC or otherwise, let us know. We'll immediately investigate the problem by testing a retained sample of your solution. If the error is on our end, you'll be offered a full refund or a free replacement – your choice. Our priority is your total satisfaction.

**Customer Satisfaction** — The primary reason we flex to your specs.

## Contents

|                               |                |
|-------------------------------|----------------|
| Potable Water Standards ..... | 72-73          |
| Wastewater Standards .....    | 74-76          |
| Custom QC Standards .....     | see pages 7-10 |

- ✓ *Traceable to NIST SRMs and lots*
- ✓ *Produced under ISO Guide 9001:2000*
- ✓ *Produced under ISO Guide 17025:2005*
- ✓ *Produced under ISO Guide 34:2000*
- ✓ *Assayed by optimal validated procedure*



Custom potable water standards are available upon request.

### Bromate

|                               |                  |
|-------------------------------|------------------|
| ICBRO31-1                     |                  |
| Volume                        | 125 mL           |
| Matrix                        | H <sub>2</sub> O |
| <b>Analyte</b>                | <b>µg/mL</b>     |
| BrO <sub>3</sub> <sup>-</sup> | 1000             |

### Bromide

|                 |                  |
|-----------------|------------------|
| ICBR1-1         |                  |
| Volume          | 125 mL           |
| Matrix          | H <sub>2</sub> O |
| <b>Analyte</b>  | <b>µg/mL</b>     |
| Br <sup>-</sup> | 1000             |

### Cation Standard

|                  |                  |
|------------------|------------------|
| QCP-CAT          |                  |
| Volume           | 20 mL            |
| Matrix           | HNO <sub>3</sub> |
| Dilution         | 1:100            |
| <b>Analyte</b>   | <b>Range</b>     |
| Ca <sup>+2</sup> | 5-200 mg/L       |
| K <sup>+</sup>   | 1-100 mg/L       |
| Mg <sup>+2</sup> | 1-200 mg/L       |
| Na <sup>+</sup>  | 6-250 mg/L       |

### Chlorate

|                               |                  |
|-------------------------------|------------------|
| ICCLO31-1                     |                  |
| Volume                        | 125 mL           |
| Matrix                        | H <sub>2</sub> O |
| <b>Analyte</b>                | <b>µg/mL</b>     |
| ClO <sub>3</sub> <sup>-</sup> | 1000             |

### Chlorite

|                               |                  |
|-------------------------------|------------------|
| ICCLO21-1                     |                  |
| Volume                        | 125 mL           |
| Matrix                        | H <sub>2</sub> O |
| <b>Analyte</b>                | <b>µg/mL</b>     |
| ClO <sub>2</sub> <sup>-</sup> | 1000             |

NOTE: Contains less than 10ppm ClO<sub>3</sub><sup>-</sup>.

### Cyanide Standard

|                                  |                  |
|----------------------------------|------------------|
| QCP-CN                           |                  |
| Volume                           | 20 mL            |
| Matrix                           | H <sub>2</sub> O |
| Dilution                         | 1:200            |
| <b>Analyte</b>                   | <b>Range</b>     |
| Total Cyanide                    | 0.04-1 mg/L      |
| Free Cyanide                     | 0.02-0.5 mg/L    |
| Cyanide Amenable to Chlorination | 0.02-0.5 mg/L    |

### Demand Standard

|                |                  |
|----------------|------------------|
| QCP-DMD        |                  |
| Volume         | 20 mL            |
| Matrix         | H <sub>2</sub> O |
| Dilution       | 1:200            |
| <b>Analyte</b> | <b>Range</b>     |
| TOC            | 6-200 mg/L       |
| COD            | 15-450 mg/L      |
| CBOD           | 15-300 mg/L      |
| BOD            | 15-300 mg/L      |

### Hg Standard

|                |                  |
|----------------|------------------|
| QCP-HG         |                  |
| Volume         | 20 mL            |
| Matrix         | HNO <sub>3</sub> |
| Dilution       | 1:200            |
| <b>Analyte</b> | <b>Range</b>     |
| Hg             | 0.5-30 µg/L      |

Used in conjunction with QCP-TMS and QCP-MTL.

### Water Hardness Standard

|                               |                                   |
|-------------------------------|-----------------------------------|
| QCP-WH                        |                                   |
| Volume                        | 500 mL                            |
| Matrix                        | H <sub>2</sub> O/HNO <sub>3</sub> |
| Dilution                      | Ready to use                      |
| <b>Analyte</b>                | <b>Range</b>                      |
| Ca                            | 3.5-150 mg/L                      |
| Mg                            | 0.9-50 mg/L                       |
| Hardness as CaCO <sub>3</sub> | 45-575 mg/L                       |

Custom potable water standards are available upon request.

### Metals Standard

|          |                  |
|----------|------------------|
| QCP-MTL  |                  |
| Volume   | 20 mL            |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:200            |

| Analyte | Range         |
|---------|---------------|
| Ag      | 4-500 µg/L    |
| Al      | 40-2000 µg/L  |
| As      | 4-500 µg/L    |
| Ba      | 40-2000 µg/L  |
| Be      | 4-500 µg/L    |
| Ca      | 30-75 mg/L    |
| Cd      | 4-500 µg/L    |
| Cr      | 40-2000 µg/L  |
| Cu      | 40-2000 µg/L  |
| Fe      | 40-2000 µg/L  |
| Mn      | 40-2000 µg/L  |
| Ni      | 40-2000 µg/L  |
| Pb      | 2-250 µg/L    |
| Sb      | 4-500 µg/L    |
| Se      | 4-500 µg/L    |
| Tl      | 4-500 µg/L    |
| Zn      | 100-1000 µg/L |

### Minerals Standard

|          |                  |
|----------|------------------|
| QCP-MIN  |                  |
| Volume   | 500 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte                       | Range         |
|-------------------------------|---------------|
| Cl <sup>-</sup>               | 10-250 mg/L   |
| F <sup>-</sup>                | 0.2-10 mg/L   |
| K <sup>+</sup>                | 2.6-150 mg/L  |
| Nitrate as N                  | 0.5-10 mg/L   |
| Conductivity                  | 50-1050 µmhos |
| Alkalinity                    | 10-150 mg/L   |
| Na <sup>+</sup>               | 7-300 mg/L    |
| SO <sub>4</sub> <sup>-2</sup> | 5-150 mg/L    |

### Nitrite Standard

|          |                  |
|----------|------------------|
| QCP-NT   |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100            |

| Analyte      | Range      |
|--------------|------------|
| Nitrite as N | 0.1-2 mg/L |

### pH Standard

|          |                  |
|----------|------------------|
| QCP-PH   |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100            |

| Analyte | Range      |
|---------|------------|
| pH      | 5-10 units |

### Simple Nutrients Standard

|           |                  |
|-----------|------------------|
| QCP-NUT-1 |                  |
| Volume    | 20 mL            |
| Matrix    | H <sub>2</sub> O |
| Dilution  | 1:200            |

| Analyte                   | Range        |
|---------------------------|--------------|
| Phosphate as P            | 0.05-10 mg/L |
| Nitrate plus Nitrite as N | 0.25-40 mg/L |
| Nitrate as N              | 0.25-40 mg/L |
| Ammonium as N             | 0.25-20 mg/L |

### Simulated Rainwater Standard

|          |                  |
|----------|------------------|
| QCP-RAIN |                  |
| Volume   | 125 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte                       | Range         |
|-------------------------------|---------------|
| Ca <sup>+2</sup>              | 0.05-0.5 mg/L |
| Cl <sup>-</sup>               | 0.1-5 mg/L    |
| F <sup>-</sup>                | 0.05-1 mg/L   |
| K <sup>+</sup>                | 0.05-1 mg/L   |
| Mg <sup>+2</sup>              | 0.05-0.5 mg/L |
| pH                            | 3.5-4.5 units |
| Conductivity                  | 20-120 µmhos  |
| Na <sup>+</sup>               | 0.2-2 mg/L    |
| NH <sub>4</sub> <sup>+</sup>  | 0.1-1.5 mg/L  |
| NO <sub>3</sub> <sup>-</sup>  | 0.1-10 mg/L   |
| SO <sub>4</sub> <sup>-2</sup> | 1-12 mg/L     |

### Total Residual Chlorine Standard

|          |                  |
|----------|------------------|
| QCP-TRC  |                  |
| Volume   | 10 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:200            |

| Analyte                 | Range       |
|-------------------------|-------------|
| Total Residual Chlorine | 0.15-5 mg/L |

### Turbidity Standard

|          |                  |
|----------|------------------|
| QCP-TURB |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100            |

| Analyte   | Range      |
|-----------|------------|
| Turbidity | 0.3-40 NTU |

Custom wastewater standards are available upon request.

### Cation Standard

|          |                  |
|----------|------------------|
| QCP-CAT  |                  |
| Volume   | 20 mL            |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte          | Range      |
|------------------|------------|
| Ca <sup>+2</sup> | 5-200 mg/L |
| K <sup>+</sup>   | 1-100 mg/L |
| Mg <sup>+2</sup> | 1-200 mg/L |
| Na <sup>+</sup>  | 6-250 mg/L |

### Chromium<sup>+6</sup> Standard

|          |                  |
|----------|------------------|
| QCP-CR6  |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100            |

| Analyte          | Range        |
|------------------|--------------|
| Cr <sup>+6</sup> | 10-1000 µg/L |

### Complex Nutrients Standard

|           |                  |
|-----------|------------------|
| QCP-NUT-2 |                  |
| Volume    | 20 mL            |
| Matrix    | H <sub>2</sub> O |
| Dilution  | 1:200            |

| Analyte                       | Range        |
|-------------------------------|--------------|
| Total Organic Phosphorus as P | 0.15-10 mg/L |
| Total Kjeldahl Nitrogen as N  | 0.35-35 mg/L |

### Cyanide Standard

|          |                  |
|----------|------------------|
| QCP-CN   |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:200            |

| Analyte                          | Range         |
|----------------------------------|---------------|
| Total Cyanide                    | 0.04-1 mg/L   |
| Free Cyanide                     | 0.02-0.5 mg/L |
| Cyanide Amenable to Chlorination | 0.02-0.5 mg/L |

### Demand Standard

|          |                  |
|----------|------------------|
| QCP-DMD  |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:200            |

| Analyte | Range       |
|---------|-------------|
| TOC     | 6-200 mg/L  |
| COD     | 15-450 mg/L |
| CBOD    | 15-300 mg/L |
| BOD     | 15-300 mg/L |

### Hardness Standard

|          |                                   |
|----------|-----------------------------------|
| QCP-WH   |                                   |
| Volume   | 500 mL                            |
| Matrix   | H <sub>2</sub> O/HNO <sub>3</sub> |
| Dilution | Ready to use                      |

| Analyte                       | Range        |
|-------------------------------|--------------|
| Ca                            | 3.5-150 mg/L |
| Mg                            | 0.9-50 mg/L  |
| Hardness as CaCO <sub>3</sub> | 45-575 mg/L  |

## Accredited...

Our laboratory often needs multi-element quality control standards to validate the analyses we provide. Unfortunately, governing bodies can't quite agree on what the standard should be. We utilize Inorganic Ventures to help us meet the specifications of each governing body and still keep our turnaround time for analyses low.

*David Rogers*  
Taylorsville, UT

Custom wastewater standards are available upon request.

### Hg Standard

|          |                  |
|----------|------------------|
| QCP-HG   |                  |
| Volume   | 20 mL            |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:200            |

| Analyte | Range |
|---------|-------|
|---------|-------|

|    |             |
|----|-------------|
| Hg | 0.5-30 µg/L |
|----|-------------|

Used in conjunction with QCP-TMS and QCP-MTL.

### Minerals Standard

|          |                  |
|----------|------------------|
| QCP-MIN  |                  |
| Volume   | 500 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte | Range |
|---------|-------|
|---------|-------|

|                               |               |
|-------------------------------|---------------|
| Cl <sup>-</sup>               | 10-250 mg/L   |
| F <sup>-</sup>                | 0.2-10 mg/L   |
| K <sup>+</sup>                | 2.6-150 mg/L  |
| Nitrate as N                  | 0.5-10 mg/L   |
| Conductivity                  | 50-1050 µmhos |
| Alkalinity                    | 10-150 mg/L   |
| Na <sup>+</sup>               | 7-300 mg/L    |
| SO <sub>4</sub> <sup>-2</sup> | 5-150 mg/L    |

### Oil & Grease Standard 1

|          |         |
|----------|---------|
| QCP-OG-A |         |
| Volume   | 20 mL   |
| Matrix   | Acetone |
| Dilution | 1:100   |

| Analyte | Range |
|---------|-------|
|---------|-------|

|              |            |
|--------------|------------|
| Oil & Grease | 8-150 mg/L |
|--------------|------------|

Applicable to gravimetric methods only.

### Oil & Grease Standard 2

|          |                  |
|----------|------------------|
| QCP-OG-W |                  |
| Volume   | 250 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte | Range |
|---------|-------|
|---------|-------|

|              |            |
|--------------|------------|
| Oil & Grease | 8-150 mg/L |
|--------------|------------|

### pH Standard

|          |                  |
|----------|------------------|
| QCP-PH   |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte | Range |
|---------|-------|
|---------|-------|

|    |            |
|----|------------|
| pH | 5-10 units |
|----|------------|

### Phenolics Standard

|          |                  |
|----------|------------------|
| QCP-PHEN |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:200            |

| Analyte | Range |
|---------|-------|
|---------|-------|

|                 |             |
|-----------------|-------------|
| Total Phenolics | 0.02-5 mg/L |
|-----------------|-------------|

### Simple Nutrients Standard

|           |                  |
|-----------|------------------|
| QCP-NUT-1 |                  |
| Volume    | 20 mL            |
| Matrix    | H <sub>2</sub> O |
| Dilution  | 1:200            |

| Analyte | Range |
|---------|-------|
|---------|-------|

|                           |              |
|---------------------------|--------------|
| Phosphate as P            | 0.05-10 mg/L |
| Nitrate plus Nitrite as N | 0.25-40 mg/L |
| Nitrate as N              | 0.25-40 mg/L |
| Ammonium as N             | 0.25-20 mg/L |

### Cooperative...

Inorganic Ventures is always willing to meet my needs or specifications. They put the customer first and always produce quality products that meet or exceed my expectations.

*Stephen Gahan*  
Covington, GA

Custom wastewater standards are available upon request.

### Solids Standard

|          |                  |
|----------|------------------|
| QCP-SLD  |                  |
| Volume   | 450 mL           |
| Matrix   | H <sub>2</sub> O |
| Dilution | Ready to use     |

| Analyte                                  | Range        |
|--|--------------|
| Total Solids (total residue)             | 70-5200 mg/L |
| Suspended Solids (nonfilterable residue) | 20-200 mg/L  |
| Dissolved Solids (filterable residue)    | 50-5000 mg/L |

### Total Residual Chlorine Standard

|          |                  |
|----------|------------------|
| QCP-TRC  |                  |
| Volume   | 10 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:200            |

| Analyte                 | Range       |
|-------------------------|-------------|
| Total Residual Chlorine | 0.15-5 mg/L |

### Experienced...

For custom-mixed standards, I'll tell Inorganic Ventures what I want, and they make it happen. I trust their expertise when it comes to putting compatible elements together. They give me the highest quality product at the best price.

*David Johnson  
Muskegon, MI*

### Trace Metals Standard

|          |                  |
|----------|------------------|
| QCP-TMS  |                  |
| Volume   | 20 mL            |
| Matrix   | HNO <sub>3</sub> |
| Dilution | 1:100            |

| Analyte | Range           |
|---------|-----------------|
| Ag      | 20-600 µg/L     |
| Al      | 100-4000 µg/L   |
| As      | 20-900 µg/L     |
| B       | 50-1000 µg/L    |
| Ba      | 100-2500 µg/L   |
| Be      | 8-900 µg/L      |
| Cd      | 8-750 µg/L      |
| Co      | 28-1000 µg/L    |
| Cr      | 17-1000 µg/L    |
| Cu      | 18-1000 µg/L    |
| Fe      | 30-4000 µg/L    |
| Mn      | 70-4000 µg/L    |
| Mo      | 24-1000 µg/L    |
| Ni      | 80-3000 µg/L    |
| Pb      | 70-3000 µg/L    |
| Sb      | 20-900 µg/L     |
| Se      | 20-2000 µg/L    |
| Sr      | 3.5-1000 µg/L   |
| Tl      | 20-900 µg/L     |
| V       | 100-10,000 µg/L |
| Zn      | 30-2000 µg/L    |

### Turbidity Standard

|          |                  |
|----------|------------------|
| QCP-TURB |                  |
| Volume   | 20 mL            |
| Matrix   | H <sub>2</sub> O |
| Dilution | 1:100            |

| Analyte   | Range      |
|-----------|------------|
| Turbidity | 0.3-40 NTU |

*"For over 20 years, getting to know our customers has been just as important as knowing how to manufacture a flawless standard."*

**Michael Scott**  
Executive Vice President





At times, Wet Chemistry involves some difficult and unusual techniques. If you find yourself in a bind, give us a call. One of our experts will be happy to assist you. Plus, we offer analytical advice and in-depth technical guides on our website, [www.inorganicventures.com](http://www.inorganicventures.com).

**Shared Knowledge** — The most rewarding part of how we flex to your specs.

## Contents

|  |       |
|--|-------|
| Wet Chemical Standards .....               | 78    |
| Sample Preparation.....                    | 79-81 |
| Custom Wet Chemistry Solutions...see pages | 7-10  |

- ✓ **Traceable to NIST SRMs and lots\***
- ✓ **Produced under ISO Guide 9001:2000**
- ✓ **Produced under ISO Guide 17025:2005\***
- ✓ **Produced under ISO Guide 34:2000\***
- ✓ **Assayed by optimal validated procedure\***

\*Not applicable for sample preparation products.



## Conductivity Standards

Custom conductivity standards are available upon request.

### 2 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON2-25

Volume 125 mL  
Matrix H<sub>2</sub>O

**NEW**

### 1200 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON1200-25

Volume 125 mL  
Matrix H<sub>2</sub>O

**NEW**

### 10 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON10-25

Volume 125 mL  
Matrix H<sub>2</sub>O

### 1400 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON1400-25

Volume 125 mL  
Matrix H<sub>2</sub>O

### 100 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON100-25

Volume 125 mL  
Matrix H<sub>2</sub>O

### 1430 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON1430-25

Volume 125 mL  
Matrix H<sub>2</sub>O

**NEW**

### 147 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON147-25

Volume 125 mL  
Matrix H<sub>2</sub>O

**NEW**

### 10,000 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON10000-25

Volume 125 mL  
Matrix H<sub>2</sub>O

### 500 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON500-25

Volume 125 mL  
Matrix H<sub>2</sub>O

**NEW**

### 100,000 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON100000-25

Volume 125 mL  
Matrix H<sub>2</sub>O

### 1000 $\mu\text{mhos/cm}$ Conductivity at 25 °C

CON1000-25

Volume 125 mL  
Matrix H<sub>2</sub>O

## Cyanide Standards

Custom cyanide standards are available upon request..

### 1000 $\mu\text{g/mL}$ Total Cyanide

CN-1000-25

Volume 20 mL  
Matrix H<sub>2</sub>O

Analyte  $\mu\text{g/mL}$

CN<sup>-</sup> 1000

## pH Calibration Standards

Custom pH calibration standards are available upon request.

### pH 2 Standard

PH-2

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 3 Standard

PH-3

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 4 Standard

PH-4

Volume 250 mL  
Matrix H<sub>2</sub>O

### pH 5 Standard

PH-5

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 6 Standard

PH-6

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 7 Standard

PH-7

Volume 250 mL  
Matrix H<sub>2</sub>O

### pH 8 Standard

PH-8

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 9 Standard

PH-9

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 10 Standard

PH-10

Volume 250 mL  
Matrix H<sub>2</sub>O

### pH 11 Standard

PH-11

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

### pH 12 Standard

PH-12

Volume 250 mL  
Matrix H<sub>2</sub>O

**NEW**

*"We always make sure our packages are delivered quickly and safely to our customers."*

**Ivy Agosto**  
Packaging Technician



## Dissolution Reagents

Designed for the preparation and measurement of samples containing silica mixed with fluoride insoluble elements, including: zeolites, alumina and/or silica based catalysts, sand, limestone, coal fly ash, and talc. The dissolution of these types of materials requires HF. See the article entitled *Elemental Analysis of Zeolites* on our website for more information.

### Acid Dissolution Reagent 1

UA-1 - 500 mL

Recommended for the dissolution of aluminosilicates, such as zeolites.

### Acid Dissolution Reagent 2<sup>†</sup>

UA-2 - 500 mL

Designed to dissolve coal fly ash and aluminosilicates.

### Acid Dissolution Reagent 3<sup>\*</sup>

UA-3 - 500 mL

Similar to UA-2, except UA-3 can handle higher levels of iron.

### Acid Dissolution Reagent 4

UA-4 - 500 mL

Designed for the dissolution of aluminosilicates, such as zeolites, containing moderate to high levels of fluoride-insoluble elements.

### Acid Dissolution Reagent 5

UA-5 - 500 mL

Designed to handle samples high in calcium, such as limestone.

### Acid Dissolution Reagent 6

UA-6 - 500 mL

Designed for samples high in magnesium, such as dolomite.

### Acid Dissolution Reagent 7

UA-7 - 500 mL

Designed for the determination of trace elements in samples containing predominately silica, such as silica gel.

<sup>†</sup>Boron cannot be determined.

<sup>\*</sup>Boron and Phosphorus cannot be determined.

## Blank Solutions

Custom blank solutions are available upon request.

### 5% (v/v) Nitric Acid Blank

IV-ACID-BLANK

|        |                  |
|--------|------------------|
| Volume | 500 mL           |
| Matrix | HNO <sub>3</sub> |

### Deionized Water Blank

IV-DI-BLANK

|        |                  |
|--------|------------------|
| Volume | 500 mL           |
| Matrix | H <sub>2</sub> O |

## Neutralizers & Stabilizers

These products are applicable to the determination of aluminosilicates containing various elements. For details, refer to the description for Dissolution Reagents on the preceding page.

### Stabilizing Reagent 1

UNS-1      2.5 L

Designed for use with UA-1.

### Stabilizing Reagent 2

UNS-2      2.5 L

Two reagent set consisting of equal amounts of UNS-2A and UNS-2B. Recommended for use with UA-2, UA-3, UA-4, or UA-5.

### Stabilizing Reagent 3

UNS-3      2.5 L

Designed for use with UA-7.

### Stabilizing Reagent 4

UNS-4      2.5 L

Prevents salting-out effects from borate fusions and/or boric acid treated HF preparations. Also recommended for use with UA-6.

### Stabilizing Reagent 100

UNS-100      2.5 L

For use with all acids and applications. Improved capacity. Contact us for more information.

### Stabilizing Reagent 300

UNS-300      2.5 L

For use with all acids and applications. Improved capacity. Contact us for more information.

## Fusion Fluxes

Custom fusion fluxes are available upon request.

### Lithium Carbonate

FF-LICO3      500 g

See section 13 of the Reliable Measurements Guide found on our website for a sample preparation method designed to work perfectly with this product.

*"Our emphasis on quality remains consistent with each customer and drives us to excel in our manufacturing efforts."*

**Jennifer Farinella**  
Manufacturing Technician



# When You Need CRMs for Environmental Analysis

*Make The Natural Choice: R.T. Corporation*

*With more than 23 years  
experience certifying  
environmental CRMs,  
RTC is the Accredited  
Specialist when it  
comes to natural soil,  
sediment, water and  
various other matrices.*



RTC's CRMs are Certified for Trace Elements, VOAs, BNAs, BTEX, TPH, PCBs, PAHs Dioxins, Pesticides and many more analytes of interest.

**RTC is the largest commercial manufacturer  
of real-world, natural-matrix CRMs.**



2931 Soldier Springs Road  
Laramie, WY 82070  
Phone: 800.576.5690 or  
307.742.5452  
Fax: 307.745.7936  
Web: [www.RT-Corp.com](http://www.RT-Corp.com)



# We flex to your specs<sup>®</sup>



Our customer service and technical support transcend the ordinary. It's truly an experience like no other. No hassles, no worries—only your complete and total satisfaction. Whether it's a custom solution or expert advice, our specialists are ready to work with you, one-on-one.



CUSTOM INORGANIC STANDARDS

### Pricing

Regional pricing may vary. Visit [www.inorganicventures.com](http://www.inorganicventures.com) for a list of current distributors.

### Shipping

Orders shipped from our European Facility in Spain are sent via FedEx or TNT. Other carriers are also available. If you prefer a specific carrier, let us know. Orders shipped out of the United States are sent FOB shipping point via UPS or Federal Express.

### Terms

Our terms are net 30 days. To establish your account, contact us during regular business hours.

### Credit Orders

We gladly accept MasterCard, Visa, or American Express.



### Cautionary Notice

OUR PRODUCTS ARE NOT FOR DRUG, FOOD OR HOUSEHOLD APPLICATIONS. They are intended for laboratory use only by qualified individuals trained in the proper handling of such materials. The consumer assumes all responsibility for the safe storage, handling, disposal and application of any Inorganic Ventures' product.

### Copyright

All content and graphics appearing herein are Copyright © 1985-2010 by Inorganic Ventures, Inc. and may not be reproduced for any purpose without Inorganic Ventures' expressed permission.

Representatives are available Monday through Friday, between 8:00 AM and 6:00 PM (EST).

**Phone:** +34.913563552 (European facility)  
1.540.585.3030 (US facility)

**Fax:** +34.913563552 (European facility)  
1.540.585.3012 (US facility)

**Email:** [iveurope@inorganicventures.com](mailto:iveurope@inorganicventures.com)

**Online:** [inorganicventures.com](http://inorganicventures.com)

### How to Order:

We have representation in more than 50 countries across the globe, including:

- Argentina
- Australia
- Belgium
- Brazil
- Canada
- China
- Ecuador
- France
- Germany
- India
- Ireland
- Italy
- Japan
- Korea
- Netherlands
- Norway
- Peru
- Scotland
- Singapore
- South Africa
- Spain
- Sweden
- Taiwan
- Thailand
- United Arab Emirates
- United Kingdom

Visit [www.inorganicventures.com/distributors](http://www.inorganicventures.com/distributors) to find the distributor in your area. Contact your distributor for regional pricing, ordering, and to request additional literature.

### Returns, Exchanges & Damaged Goods

Circumstances beyond our control may require that an item is returned or exchanged.<sup>†</sup> In such cases, a Return Authorization Number is required. Unauthorized returns will be refused. All transportation and packaging expenses on returned or exchanged items are assumed by the customer. Credit for returned items may be subject to a modest restocking fee. Credit will not be issued until it is determined by our inspection that returned items are unused and undamaged.



<sup>†</sup>Refunds, replacements and exchanges are considered at the management's discretion.

|   |                                       |
|---|---------------------------------------|
| <b>AA Standards</b>   |                                       |
| Multi-element Standards.....                                    | 70                                    |
| Single Element Standards.....                                   | 66-68                                 |
| <b>Anion Standards</b>  |                                       |
| Multi-ion Standards.....  | 61-64                                 |
| Single Ion Standards.....                                       | 58-59                                 |
| <b>Buffers</b>  |                                       |
| AA.....   | 70                                    |
| ICP & ICP-MS.....   | 34                                    |
| Calibration Blanks and Rinse Solutions.....                     | 42                                    |
| <b>Calibration Standards</b>                                    |                                       |
| AA.....   | 70                                    |
| ICP & ICP-MS.....   | 23-33, 34, 36, 38, 44, 46, 50, 52, 55 |
| Ion Chromatography.....   | 61-63                                 |
| <b>Cation Standards</b>   |                                       |
| Multi-ion Standards.....  | 61                                    |
| Potable Water Standards.....                                    | 72                                    |
| Single Ion Standards.....                                       | 60                                    |
| Wastewater Standards.....                                       | 74                                    |
| Conductivity Standards.....                                     | 64, 78                                |
| Continuing Calibration Verification Standards (CCV).....        | 35, 37, 39, 55                        |
| Contract Required Detection Limit Standards (CRDL).....         | 35, 37, 40                            |
| Contract Required Quantitation Limit Standards (CRQL).....      | 40                                    |
| Custom Standards.....   | 7-10                                  |
| <b>Cyanide Standards</b>  |                                       |
| ICP & ICP-MS.....   | 22                                    |
| Potable Water Standards.....                                    | 72                                    |
| Wastewater Standards.....                                       | 74                                    |
| Wet Chemical Testing.....                                       | 78                                    |
| Demand QC Standards.....  | 72, 74                                |
| Dissolution Reagents.....                                       | 80                                    |
| Drinking Water Standards.....                                   | 72, 73                                |
| <b>Eluents</b>  |                                       |
| for Anions.....   | 61-63                                 |
| for Cations.....  | 61                                    |
| <b>EPA Methods</b>  |                                       |
| 200.7.....  | 43-49                                 |
| 200.8.....  | 50-51                                 |
| 300.0.....  | 62                                    |
| 300.1.....  | 63-64                                 |
| 314.0.....  | 64                                    |
| 6020.....   | 52-56                                 |
| Contract Laboratory Program (CLP)                               |                                       |
| Graphite Furnace.....   | 70                                    |
| ILMO3.0.....  | 34-36                                 |
| ILMO4.0.....  | 36-38                                 |
| ILMO5.2.....  | 38-42                                 |
| ILMO5.3.....  | 38-42                                 |
| Toxicity Characteristic Leachate Procedure (TCLP).....          | 70                                    |
| Fusion Fluxes.....  | 81                                    |
| Hexavalent Chromium QC Standards.....                           | 74                                    |
| <b>ICP-OES/AES Standards</b>                                    |                                       |
| Multi-element.....  | 23-33                                 |
| Single Element.....   | 12-20                                 |
| <b>ICP-MS Standards</b>   |                                       |
| Multi-element.....  | 23-33                                 |
| Single Element.....   | 12-22                                 |
| Initial Calibration Verification Standards (ICV).....           | 35, 37, 39, 55                        |
| Interference Check Standards (ICS).....                         | 35, 37, 41, 52, 53, 55                |
| Internal Standards.....   | 42, 51, 52, 55                        |
| <b>Ion Chromatography Standards</b>                             |                                       |
| Multi-ion Standards.....  | 61-64                                 |
| Single Ion Standards.....                                       | 58-60                                 |
| Isotopic Standards.....   | 21                                    |
| Laboratory Fortifying Stock Solutions.....                      | 54, 63                                |
| Laboratory Performance Check Standards.....                     | 47, 62, 63                            |
| Matrix Modifiers.....   | 69                                    |
| Memory Check Solutions.....                                     | 52, 54, 56                            |
| Minerals QC Standards.....                                      | 73, 75                                |
| <b>Multi-element Standards</b>                                  |                                       |
| AA.....   | 70                                    |
| Calibration Standards.....                                      | 23-33, 34, 36, 38, 44, 46, 50, 52, 55 |
| ICP & ICP-MS.....   | 23-33                                 |
| Ion Chromatography.....   | 61-64                                 |
| Potable Water Standards.....                                    | 72-73                                 |
| Wastewater Standards.....                                       | 74-76                                 |
| Multi-ion Standards.....  | 61-64                                 |
| Neutralizers/Stabilizers.....                                   | 81                                    |
| <b>Nutrients QC Standards</b>                                   |                                       |
| Complex.....  | 74                                    |
| Simple.....   | 73, 75                                |
| Oil and Grease QC Standards.....                                | 75                                    |
| <b>pH Standards</b>   |                                       |
| Calibration.....  | 79                                    |
| Potable Water Standards.....                                    | 73                                    |
| Wastewater Standards.....                                       | 75                                    |
| Phenolics QC Standards.....                                     | 75                                    |
| Potable Water Standards.....                                    | 72-73                                 |
| <b>Quality Control Standards (QC)</b>                           |                                       |
| ICP & ICP-MS.....   | 44-45, 48-49, 51                      |
| Ion Chromatography.....   | 61, 64                                |
| Rainwater (Simulated).....                                      | 73                                    |
| Real World Reference Materials.....                             | 84                                    |
| Releasing Agents.....   | 69                                    |
| Sample Preparation.....   | 79-81                                 |
| <b>Single Element Standards</b>                                 |                                       |
| AA.....   | 66-68                                 |
| ICP & ICP-MS.....   | 12-20                                 |
| Single Ion Standards.....                                       | 58-60                                 |
| Soil Spike Standards.....                                       | 36, 38, 41, 53, 54, 56                |
| Solids QC Standards.....  | 76                                    |
| Speciation Standards.....                                       | 22                                    |
| Total Residual Chlorine QC Standards.....                       | 73, 76                                |
| Toxicity Characteristic Leachate Procedure Standard (TCLP)..... | 70                                    |
| Tuning Solutions.....   | 72, 51, 54, 56                        |
| Turbidity QC Standards.....                                     | 73, 76                                |
| Wastewater Standards.....                                       | 74-76                                 |
| Water Hardness QC Standard.....                                 | 72, 74                                |
| Water Spike Standards.....                                      | 36, 38, 41, 53, 54, 56                |
| Wet Chemistry Standards.....                                    | 78                                    |

# INDEX BY CATALOG NUMBER



|                      |            |              |    |                |        |                |        |
|----------------------|------------|--------------|----|----------------|--------|----------------|--------|
| 2007ICS-1.....       | 44         | AAHO1-1..... | 66 | AAU1-5.....    | 68     | CGCD1-1.....   | 14     |
| 2007ICS-3.....       | 44         | AAHO1-5..... | 66 | AAV1-1.....    | 68     | CGCD1-5.....   | 14     |
| 2007ICS-4.....       | 44         | AAIN1-1..... | 66 | AAV1-5.....    | 68     | CGCE10-1.....  | 18     |
| 2008CAL-1.....       | 50         | AAIN1-5..... | 66 | AAW1-1.....    | 68     | CGCE10-5.....  | 18     |
| 2008CAL-2.....       | 50         | AAIR1-1..... | 67 | AAW1-5.....    | 68     | CGCE1-1.....   | 14     |
| 2008ISS.....         | 51         | AAIR1-5..... | 67 | AAZ1-1.....    | 68     | CGCE1-5.....   | 14     |
| 2008TS.....          | 42, 51     | AAK1-1.....  | 67 | AAZ1-5.....    | 68     | CGCO10-1.....  | 18     |
| 300-CAL-A.....       | 62, 63     | AAK1-5.....  | 67 | AAZB1-1.....   | 68     | CGCO10-5.....  | 18     |
| 300-LFS-A.....       | 62, 63     | AALA1-1..... | 67 | AAZB1-5.....   | 68     | CGCO1-1.....   | 14     |
| 314-ANION-STOCK..... | 64         | AALA1-5..... | 67 | AAZN1-1.....   | 68     | CGCO1-5.....   | 14     |
| 6020CAL-1.....       | 52, 53, 55 | AALI1-1..... | 67 | AAZN1-5.....   | 68     | CGCR31-1.....  | 18, 22 |
| 6020ICS-0A.....      | 55         | AALI1-5..... | 67 | AAZNCN-1.....  | 22     | CGCR310-5..... | 18     |
| 6020ICS-0B.....      | 55         | AALU1-1..... | 67 | AAZNCN-5.....  | 22     | CGCR31-1.....  | 14, 22 |
| 6020ICS-8A.....      | 52         | AALU1-5..... | 67 | AAZR1-1.....   | 68     | CGCR31-5.....  | 14, 22 |
| 6020ICS-8B.....      | 52         | AAMG1-1..... | 67 | AAZR1-5.....   | 68     | CGCR61-1.....  | 14, 22 |
| 6020ICS-9A.....      | 53         | AAMG1-5..... | 67 | AGI-TS-1.....  | 32     | CGCR61-5.....  | 14, 22 |
| 6020ICS-9B.....      | 53         | AAMN1-1..... | 67 | BICARB-1.....  | 61     | CGCS10-1.....  | 18     |
| 6020ISS.....         | 52, 54, 55 | AAMN1-5..... | 67 | BICARB-5.....  | 61     | CGCS10-5.....  | 18     |
| 6020MCC-1.....       | 52, 54, 56 | AAMO1-1..... | 67 | CARB-1.....    | 61     | CGCS1-1.....   | 14     |
| 6020MCC-2.....       | 52, 54, 56 | AAMO1-5..... | 67 | CARB-5.....    | 61     | CGCS1-5.....   | 14     |
| 6020SPK-S.....       | 53, 54, 56 | AANA1-1..... | 68 | CCS-1.....     | 24     | CGCU10-1.....  | 18     |
| 6020SPK-W.....       | 53, 54, 56 | AANA1-5..... | 68 | CCS-2.....     | 24     | CGCU10-5.....  | 18     |
| 6020TS.....          | 53, 54, 56 | AANB1-1..... | 67 | CCS-4.....     | 24     | CGCU1-1.....   | 14     |
| AAAG1-1.....         | 68         | AANB1-5..... | 67 | CCS-5.....     | 24     | CGCU1-5.....   | 14     |
| AAAG1-5.....         | 68         | AAND1-1..... | 67 | CCS-6.....     | 24     | CGDY10-1.....  | 18     |
| AAAGCN-1.....        | 22         | AAND1-5..... | 67 | CG6LI1-1.....  | 15, 21 | CGDY10-5.....  | 18     |
| AAAGCN-5.....        | 22         | AANI1-1..... | 67 | CG6LI1-5.....  | 15, 21 | CGDY1-1.....   | 14     |
| AAAL1-1.....         | 66         | AANI1-5..... | 67 | CGAG10-1.....  | 20     | CGDY1-5.....   | 14     |
| AAAL1-5.....         | 66         | AAP1-1.....  | 67 | CGAG10-5.....  | 20     | CGER10-1.....  | 18     |
| AAAS1-1.....         | 66         | AAP1-5.....  | 67 | CGAG1-1.....   | 16     | CGER10-5.....  | 18     |
| AAAS1-5.....         | 66         | AAPB1-1..... | 67 | CGAG1-5.....   | 16     | CGER1-1.....   | 14     |
| AAAU1-1.....         | 66         | AAPB1-5..... | 67 | CGAL10-1.....  | 18     | CGER1-5.....   | 14     |
| AAAU1-5.....         | 66         | AAPD1-1..... | 67 | CGAL10-5.....  | 18     | CGEU10-1.....  | 18     |
| AAAUCN-1.....        | 22         | AAPD1-5..... | 67 | CGAL1-1.....   | 14     | CGEU10-5.....  | 18     |
| AAAUCN-5.....        | 22         | AAPR1-1..... | 67 | CGAL1-5.....   | 14     | CGEU1-1.....   | 14     |
| AAB1-1.....          | 66         | AAPR1-5..... | 67 | CGALCL1-1..... | 14     | CGEU1-5.....   | 14     |
| AAB1-5.....          | 66         | AAPT1-1..... | 67 | CGALCL1-5..... | 14     | CGFE10-1.....  | 19     |
| AABA1-1.....         | 66         | AAPT1-5..... | 67 | CGAS10-1.....  | 18     | CGFE10-5.....  | 19     |
| AABA1-5.....         | 66         | AARB1-1..... | 67 | CGAS10-5.....  | 18     | CGFE1-1.....   | 15     |
| AABE1-1.....         | 66         | AARB1-5..... | 67 | CGAS1-1.....   | 14     | CGFE1-5.....   | 15     |
| AABE1-5.....         | 66         | AARE1-1..... | 67 | CGAS1-5.....   | 14     | CGGA10-1.....  | 18     |
| AAB11-1.....         | 66         | AARE1-5..... | 67 | CGAS31-1.....  | 22     | CGGA10-5.....  | 18     |
| AAB11-5.....         | 66         | AARH1-1..... | 67 | CGAS31-5.....  | 22     | CGGA1-1.....   | 15     |
| AACA1-1.....         | 66         | AARH1-5..... | 67 | CGAS51-1.....  | 22     | CGGA1-5.....   | 15     |
| AACA1-5.....         | 66         | AARU1-1..... | 67 | CGAS51-5.....  | 22     | CGGD10-1.....  | 18     |
| AACD1-1.....         | 66         | AARU1-5..... | 67 | CGAU10-1.....  | 18     | CGGD10-5.....  | 18     |
| AACD1-5.....         | 66         | AAS1-1.....  | 68 | CGAU10-5.....  | 18     | CGGD1-1.....   | 15     |
| AACE1-1.....         | 66         | AAS1-5.....  | 68 | CGAU1-1.....   | 15     | CGGD1-5.....   | 15     |
| AACE1-5.....         | 66         | AASB1-1..... | 66 | CGAU1-5.....   | 15     | CGGE10-1.....  | 18     |
| AACO1-1.....         | 66         | AASB1-5..... | 66 | CGAUN1-1.....  | 15, 51 | CGGE10-5.....  | 18     |
| AACO1-5.....         | 66         | AASC1-1..... | 67 | CGAUN1-5.....  | 15     | CGGE1-1.....   | 15     |
| AACR1-1.....         | 66         | AASC1-5..... | 67 | CGB10-1.....   | 18     | CGGE1-5.....   | 15     |
| AACR1-5.....         | 66         | AASE1-1..... | 68 | CGB10-5.....   | 18     | CGHF10-1.....  | 18     |
| AACS1-1.....         | 66         | AASE1-5..... | 68 | CGB1-1.....    | 14     | CGHF10-5.....  | 18     |
| AACS1-5.....         | 66         | AASI1-1..... | 68 | CGB1-5.....    | 14     | CGHF1-1.....   | 15     |
| AACU1-1.....         | 66         | AASI1-5..... | 68 | CGBA10-1.....  | 18     | CGHF1-5.....   | 15     |
| AACU1-5.....         | 66         | AASM1-1..... | 67 | CGBA10-5.....  | 18     | CGHG10-1.....  | 19     |
| AACUCN-1.....        | 22         | AASM1-5..... | 67 | CGBA1-1.....   | 14     | CGHG10-5.....  | 19     |
| AACUCN-5.....        | 22         | AASN1-1..... | 68 | CGBA1-5.....   | 14     | CGHG1-1.....   | 15     |
| AADY1-1.....         | 66         | AASN1-5..... | 68 | CGBE10-1.....  | 18     | CGHG1-5.....   | 15     |
| AADY1-5.....         | 66         | AASR1-1..... | 68 | CGBE10-5.....  | 18     | CGHO10-1.....  | 18     |
| AAER1-1.....         | 66         | AASR1-5..... | 68 | CGBE1-1.....   | 14     | CGHO10-5.....  | 18     |
| AAER1-5.....         | 66         | AATA1-1..... | 68 | CGBE1-5.....   | 14     | CGHO1-1.....   | 15     |
| AAEU1-1.....         | 66         | AATA1-5..... | 68 | CGBI10-1.....  | 18     | CGHO1-5.....   | 15     |
| AAEU1-5.....         | 66         | AATB1-1..... | 68 | CGBI10-5.....  | 18     | CGICBR1-1..... | 14     |
| AAFE1-1.....         | 66         | AATB1-5..... | 68 | CGBI1-1.....   | 14     | CGICBR1-5..... | 14     |
| AAFE1-5.....         | 66         | AATE1-1..... | 68 | CGBI1-5.....   | 14     | CGICCL1-1..... | 14     |
| AAGA1-1.....         | 66         | AATE1-5..... | 68 | CGC10-1.....   | 18     | CGICCL1-5..... | 14     |
| AAGA1-5.....         | 66         | AATH1-1..... | 68 | CGC10-5.....   | 18     | CGIN10-1.....  | 19     |
| AAGD1-1.....         | 66         | AATH1-5..... | 68 | CGC1-1.....    | 14     | CGIN10-5.....  | 19     |
| AAGD1-5.....         | 66         | AATI1-1..... | 68 | CGC1-5.....    | 14     | CGIN1-1.....   | 15     |
| AAGE1-1.....         | 66         | AATI1-5..... | 68 | CGCA10-1.....  | 18     | CGIN1-5.....   | 15     |
| AAGE1-5.....         | 66         | AATL1-1..... | 68 | CGCA10-5.....  | 18     | CGIR10-1.....  | 19     |
| AAHF1-1.....         | 66         | AATL1-5..... | 68 | CGCA1-1.....   | 14     | CGIR10-5.....  | 19     |
| AAHF1-5.....         | 66         | AATM1-1..... | 68 | CGCA1-5.....   | 14     | CGIR1-1.....   | 15     |
| AAHG1-1.....         | 67         | AATM1-5..... | 68 | CGCD10-1.....  | 18     | CGIR1-5.....   | 15     |
| AAHG1-5.....         | 67         | AAU1-1.....  | 68 | CGCD10-5.....  | 18     | CGK10-1.....   | 19     |

|           |        |            |                    |                |            |              |            |
|-----------|--------|------------|--------------------|----------------|------------|--------------|------------|
| CGK10-5   | 19     | CGRE10-1   | 19                 | CGT10-5        | 20         | CON1400-25   | 64, 78     |
| CGK1-1    | 16     | CGRE10-5   | 19                 | CGT11-1        | 17         | CON1430-25   | 78         |
| CGK1-5    | 16     | CGRE1-1    | 16                 | CGT11-5        | 17         | CON147-25    | 78         |
| CGLA10-1  | 19     | CGRE1-5    | 16                 | CGTL10-1       | 20         | CON2-25      | 78         |
| CGLA10-5  | 19     | CGRH10-1   | 19                 | CGTL10-5       | 20         | CON500-25    | 78         |
| CGLA1-1   | 15     | CGRH10-5   | 19                 | CGTL1-1        | 17         | CRI-CRA-1    | 35, 37     |
| CGLA1-5   | 15     | CGRH1-1    | 16                 | CGTL1-5        | 17         | CRI-CRA-2    | 35, 37     |
| CGLI10-1  | 19     | CGRH1-5    | 16                 | CGTM10-1       | 20         | CRI-CRA-3    | 35, 37     |
| CGLI10-5  | 19     | CGRHN1-1   | 16                 | CGTM10-5       | 20         | CSN-ISB-5    | 34         |
| CGLI1-1   | 15, 21 | CGRHN1-5   | 16                 | CGTM1-1        | 17         | CSN-ISB5-5   | 34         |
| CGLI1-5   | 15, 21 | CGRU10-1   | 19                 | CGTM1-5        | 17         | ELUENT1817-1 | 61, 62, 63 |
| CGLU10-1  | 19     | CGRU10-5   | 19                 | CGU10-1        | 20         | ELUENT1817-5 | 61, 62, 63 |
| CGLU10-5  | 19     | CGRU1-1    | 16                 | CGU10-5        | 20         | ELUENT3510-1 | 61         |
| CGLU1-1   | 15     | CGRU1-5    | 16                 | CGU1-1         | 17         | ELUENT3510-5 | 61         |
| CGLU1-5   | 15     | CGS10-1    | 20                 | CGU1-5         | 17         | FF-LICO3     | 81         |
| CGMG10-1  | 19     | CGS10-5    | 20                 | CGV10-1        | 20         | GENESIS-CAL  | 26         |
| CGMG10-5  | 19     | CGS1-1     | 17                 | CGV10-5        | 20         | ICADP1-1     | 58         |
| CGMG1-1   | 15     | CGS1-5     | 17                 | CGV1-1         | 17         | ICADP1-5     | 58         |
| CGMG1-5   | 15     | CGSB10-1   | 18                 | CGV1-5         | 17         | ICBA1-1      | 60         |
| CGMN10-1  | 19     | CGSB10-5   | 18                 | CGW10-1        | 20         | ICBA1-5      | 60         |
| CGMN10-5  | 19     | CGSB1-1    | 14, 34, 36, 38, 44 | CGW10-5        | 20         | ICBEN1-1     | 58         |
| CGMN1-1   | 15     | CGSB1-5    | 14                 | CGW1-1         | 17         | ICBEN1-5     | 58         |
| CGMN1-5   | 15     | CGSBF1-1   | 14                 | CGW1-5         | 17         | ICBR1-1      | 58, 64, 72 |
| CGMO10-1  | 19     | CGSBF1-5   | 14                 | CGY10-1        | 20         | ICBR1-5      | 58         |
| CGMO10-5  | 19     | CGSC10-1   | 20                 | CGY10-5        | 20         | ICBRO31-1    | 58, 64, 72 |
| CGMO1-1   | 15     | CGSC10-5   | 20                 | CGY1-1         | 17         | ICBRO31-5    | 58         |
| CGMO1-5   | 15     | CGSC1-1    | 16                 | CGY1-5         | 17         | ICBTR1-1     | 58         |
| CGMSA10-1 | 20     | CGSC1-5    | 16                 | CGYB10-1       | 20         | ICBTR1-5     | 58         |
| CGMSA10-5 | 20     | CGSE10-1   | 20                 | CGYB10-5       | 20         | ICCA1-1      | 60         |
| CGMSA1-1  | 16     | CGSE10-5   | 20                 | CGYB1-1        | 17         | ICCA1-5      | 60         |
| CGMSA1-5  | 16     | CGSE41-1   | 16, 22             | CGYB1-5        | 17         | ICCT1-1      | 58         |
| CGNA10-1  | 20     | CGSE41-5   | 16, 22             | CGZN10-1       | 20         | ICCT1-5      | 58         |
| CGNA10-5  | 20     | CGSE61-1   | 22                 | CGZN10-5       | 20         | ICCL1-1      | 58         |
| CGNA1-1   | 16     | CGSE61-5   | 22                 | CGZN1-1        | 17         | ICCL1-5      | 58         |
| CGNA1-5   | 16     | CGSI10-1   | 20                 | CGZN1-5        | 17         | ICCLO21-1    | 58, 64, 72 |
| CGNB10-1  | 19     | CGSI10-5   | 20                 | CGZR10-1       | 20         | ICCLO21-5    | 58         |
| CGNB10-5  | 19     | CGSI1-1    | 16                 | CGZR10-5       | 20         | ICCLO31-1    | 58, 64, 72 |
| CGNB1-1   | 15     | CGSI1-5    | 16                 | CGZR1-1        | 17         | ICCLO31-5    | 58         |
| CGNB1-5   | 15     | CGSINA1-1  | 16                 | CGZR1-5        | 17         | ICCLO41-1    | 59         |
| CGND10-1  | 19     | CGSINA1-5  | 16                 | CIROS-OES-TS   | 32         | ICCLO41-5    | 59         |
| CGND10-5  | 19     | CGSIO1-1   | 16                 | CLP-AES-CRDL   | 40         | ICCO31-1     | 58         |
| CGND1-1   | 15     | CGSIO1-5   | 16                 | CLP-AES-CRQL   | 40         | ICCO31-5     | 58         |
| CGND1-5   | 15     | CGSIONA1-1 | 16                 | CLP-AES-CRQL-2 | 40         | ICCRO41-1    | 58         |
| CGNI10-1  | 19     | CGSIONA1-5 | 16                 | CLPF-ASPK-1    | 70         | ICCRO41-5    | 58         |
| CGNI10-5  | 19     | CGSM10-1   | 20                 | CLPF-CAL-1     | 70         | ICCS1-1      | 60         |
| CGNI1-1   | 15     | CGSM10-5   | 20                 | CLPF-PSPK-1    | 70         | ICCS1-5      | 60         |
| CGNI1-5   | 15     | CGSM1-1    | 16                 | CLP-MS-BLANK   | 42         | ICDCA-S-1    | 63, 64     |
| CGOS1-1   | 16     | CGSM1-5    | 16                 | CLP-MS-CAL     | 38         | ICDCA-S-5    | 63, 64     |
| CGOS1-5   | 16     | CGSN10-1   | 20                 | CLP-MS-CICV    | 39         | ICDEA1-1     | 60         |
| CGP10-1   | 19     | CGSN10-5   | 20                 | CLP-MS-CRQL    | 40         | ICDEA1-5     | 60         |
| CGP10-5   | 19     | CGSN1-1    | 17                 | CLP-MS-CRQL-2  | 40         | ICDMA1-1     | 60         |
| CGP1-1    | 16     | CGSN1-5    | 17                 | CLP-MS-CRQL-3  | 40         | ICDMA1-5     | 60         |
| CGP1-5    | 16     | CGSNCL1-1  | 17                 | CLP-MS-ICS-B   | 41         | ICF1-1       | 58         |
| CGPB10-1  | 19     | CGSNCL1-5  | 17                 | CLP-MS-RINSE   | 42         | ICF1-5       | 58         |
| CGPB10-5  | 19     | CGSR10-1   | 20                 | CLP-MS-SPK     | 41         | IC-FAS-1A    | 61         |
| CGPB1-1   | 15     | CGSR10-5   | 20                 | CLPP-CAL-1     | 34, 36, 38 | ICGLY1-1     | 58         |
| CGPB1-5   | 15     | CGSR1-1    | 16                 | CLPP-CAL-3     | 34, 36, 38 | ICGLY1-5     | 58         |
| CGPD10-1  | 19     | CGSR1-5    | 16                 | CLPP-ICS-A     | 35, 37, 41 | ICGTR1-1     | 58         |
| CGPD10-5  | 19     | CGTA10-1   | 20                 | CLPP-ICS-B     | 35         | ICGTR1-5     | 58         |
| CGPD1-1   | 16     | CGTA10-5   | 20                 | CLPP-ICS-B4    | 37, 41     | ICHCO1-1     | 58         |
| CGPD1-5   | 16     | CGTA1-1    | 17                 | CLPP-SPK-1     | 36, 38, 41 | ICHCO1-5     | 58         |
| CGPDN1-1  | 16     | CGTA1-5    | 17                 | CLPP-SPK-2     | 36, 43, 46 | ICI1-1       | 15, 58     |
| CGPDN1-5  | 16     | CGTB10-1   | 20                 | CLPP-SPK-3     | 36         | ICI1-5       | 15, 58     |
| CGPR10-1  | 19     | CGTB10-5   | 20                 | CLPP-SPK-4     | 38         | ICK1-1       | 60         |
| CGPR10-5  | 19     | CGTB1-1    | 17                 | CLPP-SPK-5     | 41         | ICK1-5       | 60         |
| CGPR1-1   | 16     | CGTB1-5    | 17                 | CMS-1          | 23         | ICKHP1-1     | 59         |
| CGPR1-5   | 16     | CGTE10-1   | 20                 | CMS-2          | 23         | ICKHP1-5     | 59         |
| CGPT10-1  | 19     | CGTE10-5   | 20                 | CMS-3          | 23         | ICLCT1-1     | 58         |
| CGPT10-5  | 19     | CGTE1-1    | 17                 | CMS-4          | 23         | ICLCT1-5     | 58         |
| CGPT1-1   | 16     | CGTE1-5    | 17                 | CMS-5          | 23         | ICLI1-1      | 60         |
| CGPT1-5   | 16     | CGTEN1-1   | 17                 | CN-1000-25     | 78         | ICLI1-5      | 60         |
| CGPTN1-1  | 16     | CGTEN1-5   | 17                 | CON100000-25   | 78         | ICMEA1-1     | 60         |
| CGPTN1-5  | 16     | CGTH10-1   | 20                 | CON10000-25    | 78         | ICMEA1-5     | 60         |
| CGRB10-1  | 19     | CGTH10-5   | 20                 | CON1000-25     | 78         | ICMG1-1      | 60         |
| CGRB10-5  | 19     | CGTH1-1    | 17                 | CON100-25      | 78         | ICMG1-5      | 60         |
| CGRB1-1   | 16     | CGTH1-5    | 17                 | CON10-25       | 78         | ICMLA1-1     | 58         |
| CGRB1-5   | 16     | CGTI10-1   | 20                 | CON1200-25     | 78         | ICMLA1-5     | 58         |

|                    |        |                    |        |                   |        |                   |            |
|--------------------|--------|--------------------|--------|-------------------|--------|-------------------|------------|
| ICMLE1-1.....      | 58     | IV-STOCK-8.....    | 27     | MSCD-100PPM.....  | 13     | PH-10.....        | 79         |
| ICMLE1-5.....      | 58     | IV-STOCK-9.....    | 28     | MSCD-10PPM.....   | 12     | PH-11.....        | 79         |
| ICMLO1-1.....      | 58     | IV-STOCK-10.....   | 28     | MSCO-100PPM.....  | 13     | PH-12.....        | 79         |
| ICMLO1-5.....      | 58     | IV-STOCK-11.....   | 28     | MSCO-10PPM.....   | 12     | PH-2.....         | 79         |
| ICMMA1-1.....      | 60     | IV-STOCK-12.....   | 33     | MSCR3-100PPM..... | 13     | PH-3.....         | 79         |
| ICMMA1-5.....      | 60     | IV-STOCK-13.....   | 28     | MSCR3-10PPM.....  | 12     | PH-4.....         | 79         |
| ICMPA1-1.....      | 60     | IV-STOCK-14.....   | 32     | MSCR6-100PPM..... | 13     | PH-5.....         | 79         |
| ICMPA1-5.....      | 60     | IV-STOCK-15.....   | 29     | MSCR6-10PPM.....  | 12     | PH-6.....         | 79         |
| ICMSA1-1.....      | 58     | IV-STOCK-16.....   | 28     | MSCS-100PPM.....  | 13     | PH-7.....         | 79         |
| ICMSA1-5.....      | 58     | IV-STOCK-1643..... | 31     | MSCS-10PPM.....   | 12     | PH-8.....         | 79         |
| ICNA1-1.....       | 60     | IV-STOCK-17.....   | 29     | MSCU-100PPM.....  | 13     | PH-9.....         | 79         |
| ICNA1-5.....       | 60     | IV-STOCK-18.....   | 69     | MSCU-10PPM.....   | 12     | QCP-CAT.....      | 72, 74     |
| ICNH41-1.....      | 60     | IV-STOCK-19.....   | 31     | MSFE-100PPM.....  | 13     | QCP-CICV-1.....   | 35, 37, 39 |
| ICNH41-5.....      | 60     | IV-STOCK-20.....   | 31     | MSFE-10PPM.....   | 12     | QCP-CICV-2.....   | 35, 37, 39 |
| ICNNH41-1.....     | 60     | IV-STOCK-21.....   | 29     | MSGE-100PPM.....  | 13     | QCP-CICV-3.....   | 35, 37, 39 |
| ICNNH41-5.....     | 60     | IV-STOCK-22.....   | 29     | MSGE-10PPM.....   | 12     | QCP-CICV-4.....   | 70         |
| ICNNO21-1.....     | 59     | IV-STOCK-23.....   | 29     | MSHG-100PPM.....  | 13     | QCP-CN.....       | 72, 74     |
| ICNNO21-5.....     | 59     | IV-STOCK-24.....   | 33     | MSHG-10PPM.....   | 12, 25 | QCP-CR6.....      | 74         |
| ICNNO31-1.....     | 59     | IV-STOCK-25.....   | 69     | MSHGN-100PPM..... | 13     | QCP-DMD.....      | 72, 74     |
| ICNNO31-5.....     | 59     | IV-STOCK-26.....   | 29     | MSHGN-10PPM.....  | 12     | QCP-HG.....       | 72, 75     |
| ICNO21-1.....      | 59     | IV-STOCK-27.....   | 30     | MSHO-100PPM.....  | 13     | QCP-ICV-1REV..... | 39, 55     |
| ICNO21-5.....      | 59     | IV-STOCK-28.....   | 30     | MSHO-10PPM.....   | 12     | QCP-MIN.....      | 73, 75     |
| ICNO31-1.....      | 58     | IV-STOCK-29.....   | 30     | MSIN-100PPM.....  | 13     | QCP-MTL.....      | 73         |
| ICNO31-5.....      | 58     | IV-STOCK-30.....   | 30     | MSIN-10PPM.....   | 12     | QCP-NT.....       | 73         |
| ICNTA1-1.....      | 59     | IV-STOCK-31.....   | 30     | MSK-100PPM.....   | 13     | QCP-NUT-1.....    | 73, 75     |
| ICNTA1-5.....      | 59     | IV-STOCK-33.....   | 31     | MSK-10PPM.....    | 12     | QCP-NUT-2.....    | 74         |
| ICOAC1-1.....      | 58     | KN-ISB-5.....      | 34     | MSLI-100PPM.....  | 13     | QCP-OG-A.....     | 75         |
| ICOAC1-5.....      | 58     | LACB1-5.....       | 69     | MSLI-10PPM.....   | 12, 25 | QCP-OG-W.....     | 75         |
| ICOPR1-1.....      | 59     | LINB2-5.....       | 34, 69 | MSMG-100PPM.....  | 13     | QCP-PH.....       | 73, 75     |
| ICOPR1-5.....      | 59     | MM-MG-10.....      | 69     | MSMG-10PPM.....   | 12     | QCP-PHEN.....     | 75         |
| ICOX1-1.....       | 59     | MM-P-40.....       | 69     | MSMN-100PPM.....  | 13     | QCP-QCS-1.....    | 44, 48     |
| ICOX1-5.....       | 59     | MM-PD-10.....      | 69     | MSMN-10PPM.....   | 12     | QCP-QCS-2.....    | 44, 48     |
| ICPO41-1.....      | 59     | MM-PD-5.....       | 69     | MSMO-100PPM.....  | 13     | QCP-QCS-3.....    | 51         |
| ICPO41-5.....      | 59     | MM-PDMG-32.....    | 69     | MSMO-10PPM.....   | 12     | QCP-QCS-4.....    | 51         |
| ICPPO41-1.....     | 59     | MS106CD-10PPM..... | 21     | MSNA-100PPM.....  | 13     | QCP-QCS-5.....    | 62, 63     |
| ICPPO41-5.....     | 59     | MS109AG-10PPM..... | 21     | MSNA-10PPM.....   | 12     | QCP-RAIN.....     | 73         |
| ICRB1-1.....       | 60     | MS10B-10PPM.....   | 21     | MSNI-100PPM.....  | 13     | QCP-SLD.....      | 76         |
| ICRB1-5.....       | 60     | MS11B-10PPM.....   | 21     | MSNI-10PPM.....   | 12     | QCP-TMS.....      | 76         |
| ICS2O31-1.....     | 59     | MS122SN-10PPM..... | 21     | MSOS-100PPM.....  | 13     | QCP-TRC.....      | 73, 76     |
| ICS2O31-5.....     | 59     | MS135BA-10PPM..... | 21     | MSOS-10PPM.....   | 12     | QCP-TURB.....     | 73, 76     |
| ICSCC1-1.....      | 59     | MS203TL-10PPM..... | 21     | MSPB-100PPM.....  | 13     | QCP-WH.....       | 72, 74     |
| ICSCC1-5.....      | 59     | MS204PB-10PPM..... | 21     | MSPB-10PPM.....   | 12     | TCLP-1REV.....    | 70         |
| ICSCN1-1.....      | 59     | MS205TL-10PPM..... | 21     | MSRH-100PPM.....  | 13     | TCLP-AA-HG.....   | 70         |
| ICSCN1-5.....      | 59     | MS206PB-10PPM..... | 21     | MSRH-10PPM.....   | 12     | THM-TS-1.....     | 32         |
| IC-SCS1-1.....     | 61     | MS207PB-10PPM..... | 21     | MSRHN-100PPM..... | 13     | UA-1.....         | 80         |
| ICSO41-1.....      | 59     | MS25MG-10PPM.....  | 21     | MSRHN-10PPM.....  | 12     | UA-2.....         | 80         |
| ICSO41-5.....      | 59     | MS50CR-10PPM.....  | 21     | MSSB-100PPM.....  | 13     | UA-3.....         | 80         |
| ICSR1-1.....       | 60     | MS54FE-10PPM.....  | 21     | MSSB-10PPM.....   | 12     | UA-4.....         | 80         |
| ICSR1-5.....       | 60     | MS57FE-10PPM.....  | 21     | MSSC-100PPM.....  | 13     | UA-5.....         | 80         |
| ICTA1-1.....       | 60     | MS61NI-10PPM.....  | 21     | MSSC-10PPM.....   | 12     | UA-6.....         | 80         |
| ICTA1-5.....       | 60     | MS65CU-10PPM.....  | 21     | MSSE-100PPM.....  | 13     | UA-7.....         | 80         |
| ICTEA1-1.....      | 60     | MS67ZN-10PPM.....  | 21     | MSSE-10PPM.....   | 12     | UNS-1.....        | 81         |
| ICTEA1-5.....      | 60     | MS6LI-100PPM.....  | 13     | MSSN-100PPM.....  | 13     | UNS-100.....      | 81         |
| ICTMA1-1.....      | 60     | MS6LI-10PPM.....   | 12     | MSSN-10PPM.....   | 12     | UNS-2.....        | 81         |
| ICTMA1-5.....      | 60     | MS78SE-10PPM.....  | 21     | MSSR-100PPM.....  | 13     | UNS-3.....        | 81         |
| ICTMAH1-1.....     | 60     | MS82SE-10PPM.....  | 21     | MSSR-10PPM.....   | 12     | UNS-300.....      | 81         |
| ICTMAH1-5.....     | 60     | MS86SR-10PPM.....  | 21     | MSTB-100PPM.....  | 13     | UNS-4.....        | 81         |
| ICTRTR1-1.....     | 59     | MSAELUENT-1.....   | 61     | MSTB-10PPM.....   | 12     | VAR-CAL-1.....    | 26         |
| ICTRTR1-5.....     | 59     | MSAELUENT-5.....   | 61     | MSTEN-10PPM.....  | 12     | VAR-CAL-2.....    | 26         |
| IV-19.....         | 45, 49 | MSAG-100PPM.....   | 13     | MSTEN-100PPM..... | 13, 24 | VAR-CAL-7.....    | 26         |
| IV-21.....         | 45, 49 | MSAG-10PPM.....    | 12     | MSTH-100PPM.....  | 13     | VAR-IS-1.....     | 31         |
| IV-26.....         | 45, 49 | MSAL-100PPM.....   | 13     | MSTH-10PPM.....   | 12     | VAR-TS-MS.....    | 33         |
| IV-28.....         | 45, 49 | MSAL-10PPM.....    | 12     | MSTI-100PPM.....  | 13     | WW-CAL-1A.....    | 43, 46     |
| IV-7.....          | 45, 49 | MSAS-100PPM.....   | 13     | MSTI-10PPM.....   | 12     | WW-CAL-2.....     | 43, 46     |
| IV-ACID-BLANK..... | 80     | MSAS-10PPM.....    | 12     | MSTL-100PPM.....  | 13     | WW-CAL-3.....     | 43, 46     |
| IV-DI-BLANK.....   | 80     | MSAU-100PPM.....   | 13     | MSTL-10PPM.....   | 12     | WW-CAL-4A.....    | 43, 46     |
| IV-ICPMS-71A.....  | 25     | MSAU-10PPM.....    | 12     | MSU-100PPM.....   | 13     | WW-CAL-4B.....    | 43, 46     |
| IV-ICPMS-71B.....  | 25     | MSB-100PPM.....    | 13     | MSU-10PPM.....    | 12     | WW-CAL-5.....     | 43, 46     |
| IV-ICPMS-71C.....  | 25     | MSB-10PPM.....     | 12     | MSV-100PPM.....   | 13     | WW-IPC-1.....     | 47         |
| IV-ICPMS-71D.....  | 25     | MSBA-100PPM.....   | 13     | MSV-10PPM.....    | 12     | WW-IPC-2.....     | 47         |
| IV-STOCK-1.....    | 27     | MSBA-10PPM.....    | 12     | MSY-100PPM.....   | 13     | WW-IPC-3.....     | 47         |
| IV-STOCK-2.....    | 27     | MSBE-100PPM.....   | 13     | MSY-10PPM.....    | 12     | WW-LFS-1.....     | 48         |
| IV-STOCK-3.....    | 27     | MSBE-10PPM.....    | 12     | MSZN-100PPM.....  | 13     | WW-LFS-2.....     | 48         |
| IV-STOCK-4.....    | 27     | MSBI-100PPM.....   | 13     | MSZN-10PPM.....   | 12     | WW-MSCAL-1.....   | 50         |
| IV-STOCK-5.....    | 32     | MSBI-10PPM.....    | 12     | PE-CAL-3.....     | 26     | WW-MSCAL-2.....   | 50         |
| IV-STOCK-6.....    | 28     | MSCA-100PPM.....   | 13     | PE-CHK-1.....     | 31     |                   |            |
| IV-STOCK-7.....    | 61     | MSCA-10PPM.....    | 12     | PE-TS-1.....      | 32     |                   |            |

# CUSTOM STANDARD QUOTATION REQUEST FORM

Page \_\_\_\_ of \_\_\_\_

To: Sales Department  
Inorganic Ventures  
300 Technology Drive  
Christiansburg, VA 24073

- 1 Photocopy this page.
- 2 Fill out the form.
- 3 Fax to 1.540.585.3012.

From: Name \_\_\_\_\_

Date\* \_\_\_\_\_

Company \_\_\_\_\_

Account No. \_\_\_\_\_  
(optional)

Address \_\_\_\_\_

Phone \_\_\_\_\_

\_\_\_\_\_

Fax \_\_\_\_\_

## Describe your blend:

| Analyte   | Concentration | Analyte   | Concentration |
|-----------|---------------|-----------|---------------|
| 1. _____  | _____         | 21. _____ | _____         |
| 2. _____  | _____         | 22. _____ | _____         |
| 3. _____  | _____         | 23. _____ | _____         |
| 4. _____  | _____         | 24. _____ | _____         |
| 5. _____  | _____         | 25. _____ | _____         |
| 6. _____  | _____         | 26. _____ | _____         |
| 7. _____  | _____         | 27. _____ | _____         |
| 8. _____  | _____         | 28. _____ | _____         |
| 9. _____  | _____         | 29. _____ | _____         |
| 10. _____ | _____         | 30. _____ | _____         |
| 11. _____ | _____         | 31. _____ | _____         |
| 12. _____ | _____         | 32. _____ | _____         |
| 13. _____ | _____         | 33. _____ | _____         |
| 14. _____ | _____         | 34. _____ | _____         |
| 15. _____ | _____         | 35. _____ | _____         |
| 16. _____ | _____         | 36. _____ | _____         |
| 17. _____ | _____         | 37. _____ | _____         |
| 18. _____ | _____         | 38. _____ | _____         |
| 19. _____ | _____         | 39. _____ | _____         |
| 20. _____ | _____         | 40. _____ | _____         |

### Units:

- µg/mL
- µg/L
- µg/g
- µg/Kg
- mg/L
- ng/mL
- ng/g
- g/mL

### Volume:

- 125 mL
- 250 mL
- 500 mL
- 1000 mL
- \_\_\_\_\_ L
- \_\_\_\_\_ units

### Matrix:

- \_\_\_\_\_
- Inorganic Ventures can specify

Requested Delivery Date: \_\_\_\_\_

- Next-Day RUSH Manufacturing**  
Solution will arrive in 48-72 business hours  
at no additional charge.

Comments: \_\_\_\_\_

\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

You may also request quotations online:

[www.inorganicventures.com](http://www.inorganicventures.com)

\*Quotations are void 60 days after quotation date.





Calle de Villafranca, 17  
Porteria (Local 8)  
Madrid, Spain 28028  
info@inorganicventures.com



[www.inorganicventures.com](http://www.inorganicventures.com)